


Mass Spectrum

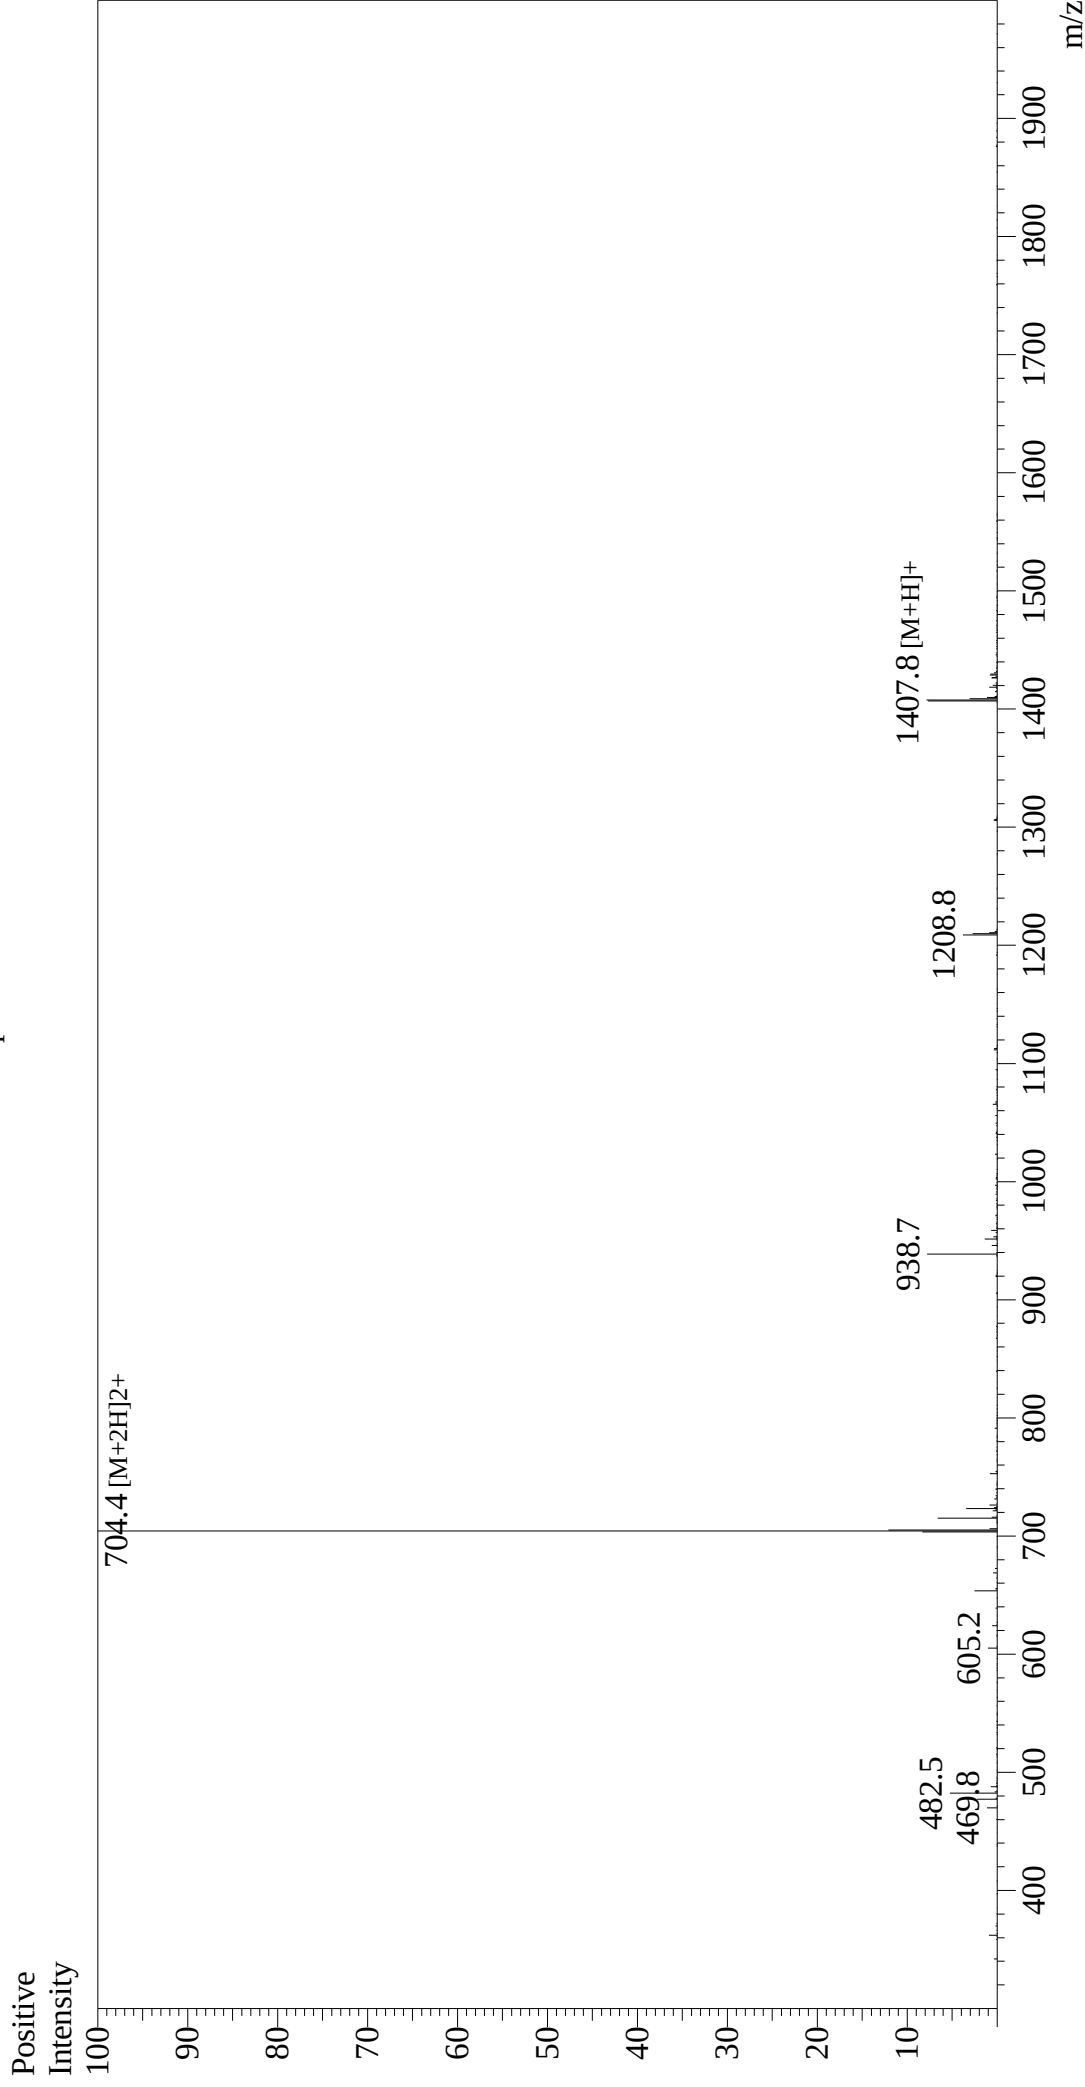

Sample Information

Month-Day Processed : 09/08/22

Time Processed : 10:30:40

Injection Volume : 0.1

Sample Name : Hepatitis B Virus Core (128-140)

Cat No. : RP17313

Lot No. : E6421522I

Theoretical MW: 1406.63

Observed MW : 1406.8

Interface

Nebulizing Gas Flow : 1.5L/min

CDL Temp : 250

Block Temp : 200

Equipment

Interface Bias

Drying Gas Flow

T.Flow

B.conc

: ZJ21010035

: +4.5 kV

: 5 L/min

: 0.2 ml/min

: 50%H₂O/50%MeOH