


Mass Spectrum

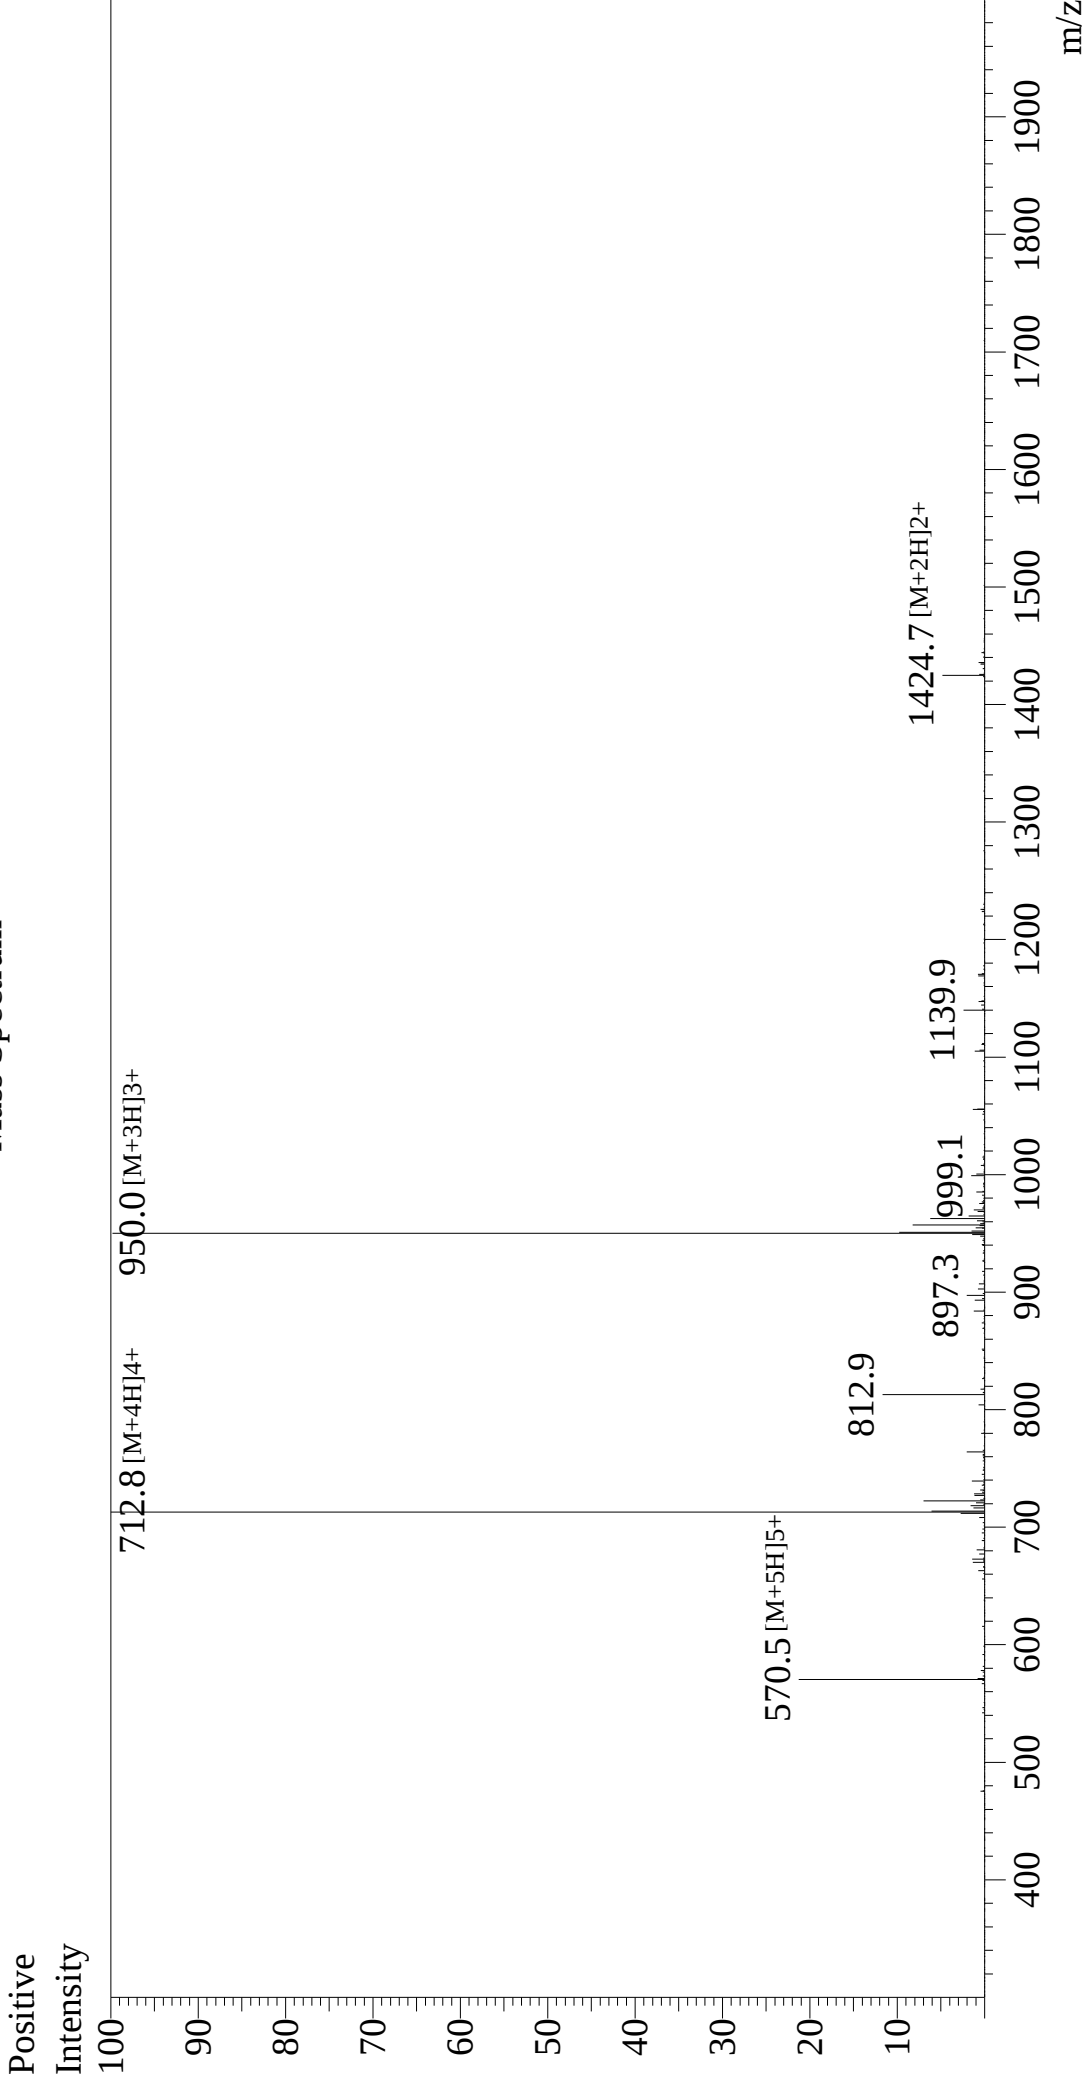

Sample Information

Month-Day Processed : 02/04/26
Time Processed : 18:52:40
Injection Volume : 0.3
Sample Name : Melittin,honey bee

Cat No. : RP20415
Lot No. : E6677326B

Theoretical MW: 2847.50

Observed MW : 2847.2

Interface

Nebulizing Gas Flow :1.5L/min
CDL Temp :250
Block Temp :200

:ESI

Interface Bias :+4.5 kV
Drying Gas Flow :5 L/min
T.Flow :0.2 ml/min
B.conc :50%H2O/50%MeOH

Equipment

: ZJ21010035