


Mass Spectrum

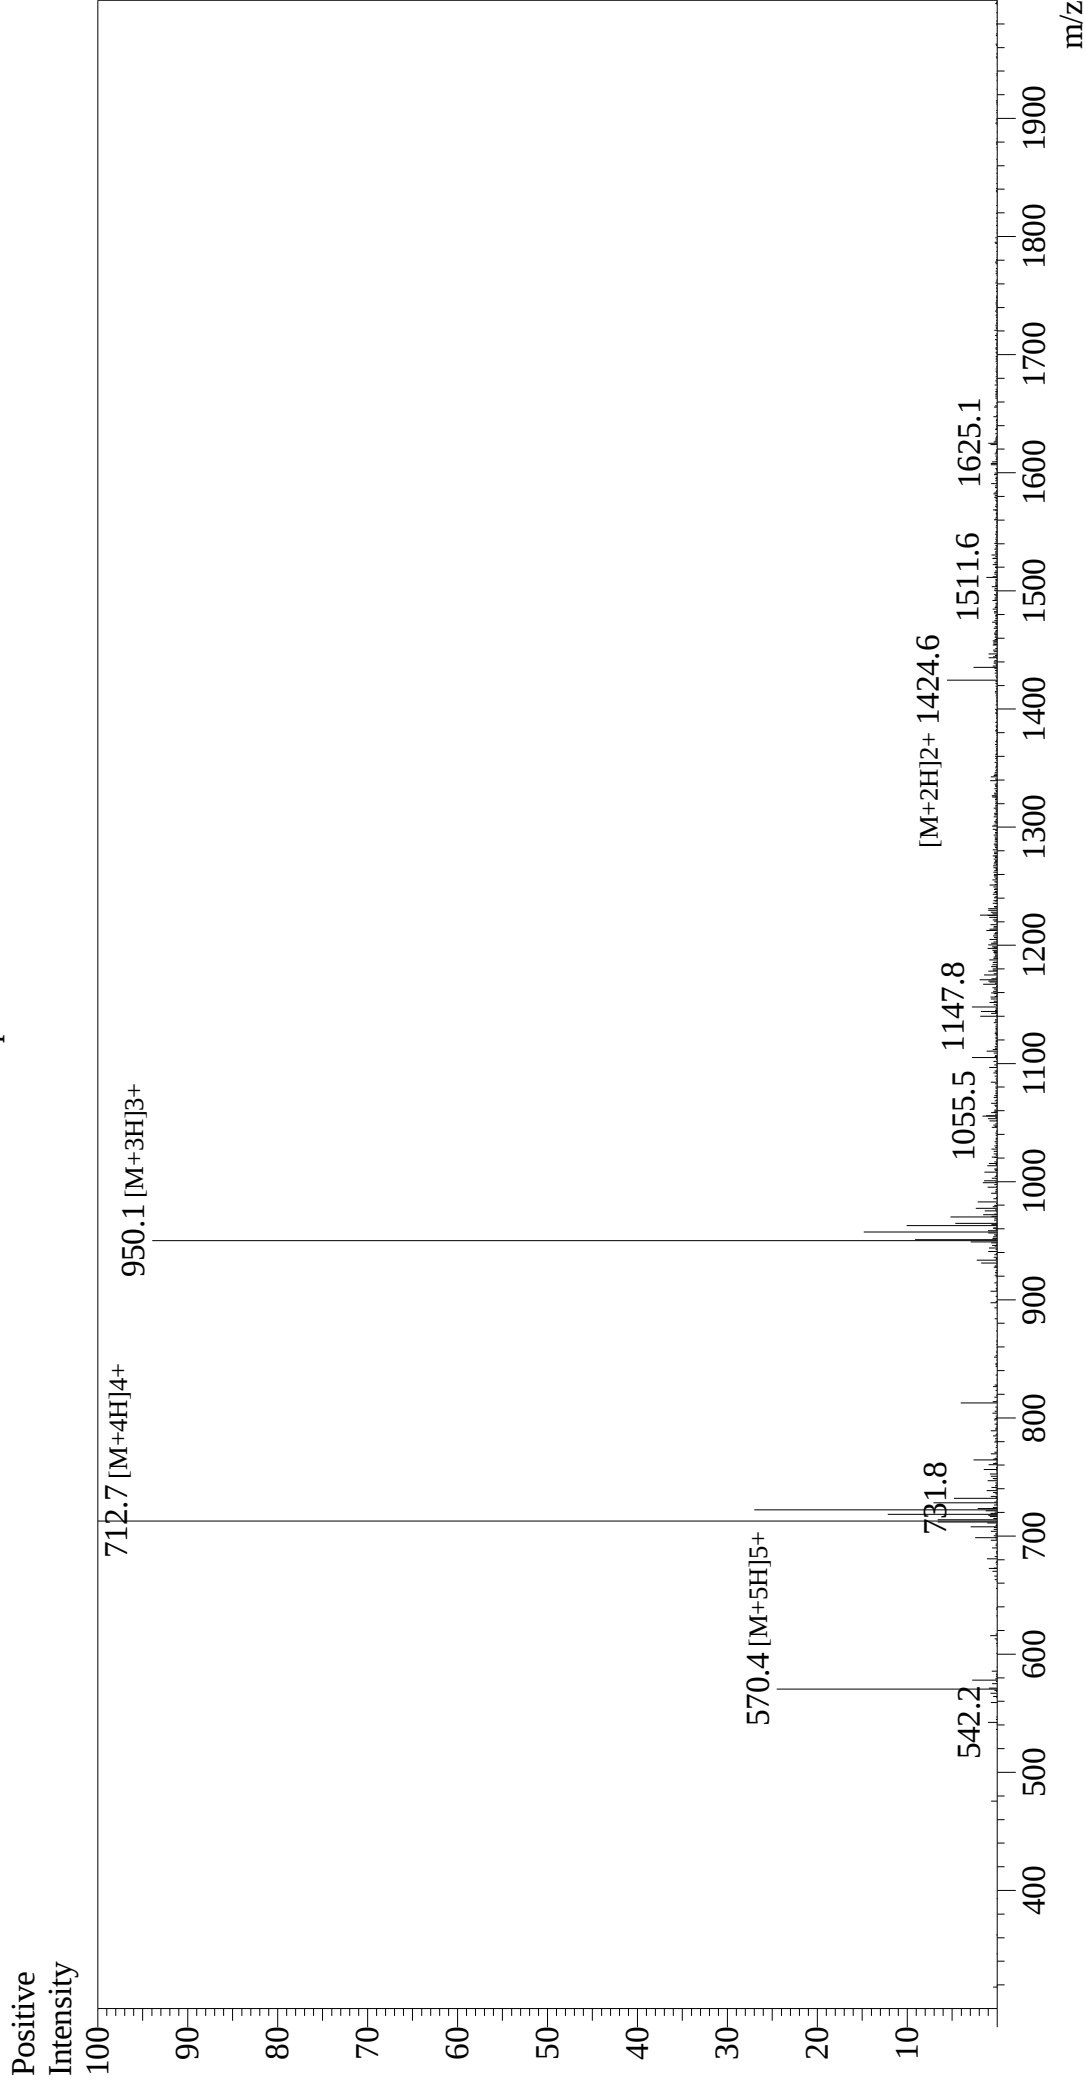

Sample Information

Month-Day Processed : 06/06/24
 Time Processed : 12:28:30
 Injection Volume : 0.4
 Sample Name : Melittin,honey bee
 Cat No. : RP20415
 Lot No. : E6762524F
 Theoretical MW: 2847.50
 Observed MW : 2846.8

Interface :ESI
 Nebulizing Gas Flow :1.5L/min
 CDL Temp :250
 Block Temp :200

Equipment :ZJ22010150
 Interface Bias :+4.5 kV
 Drying Gas Flow :5 L/min
 T.Flow :0.2 ml/min
 B.conc :50%H₂O/50%MeOH