

Sample Name : Calcitonin Gene Related Peptide (CGRP), rat

Cat No. : RP11095

Lot No. : E6765623L

Time Processed :16:09:24

Month-Day-Year Processed :02/24/2024

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm

Equipment: ZJ20010140

<Chromatogram>

mV

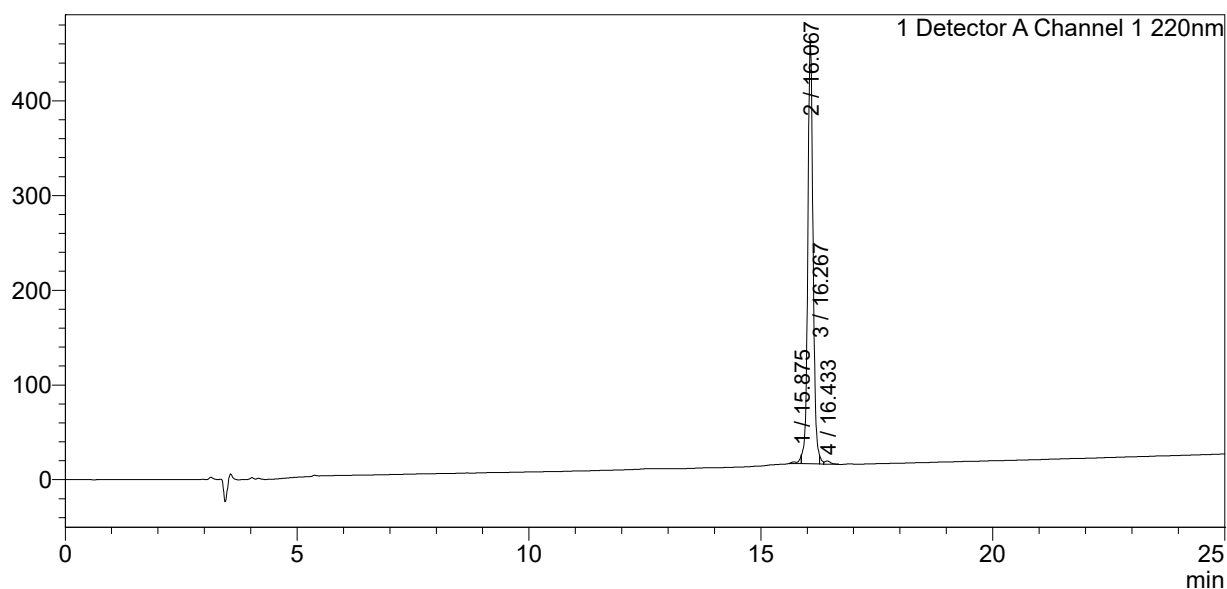

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.875	36238	9145	1.000
2	16.067	3532498	446897	97.519
3	16.267	25015	9326	0.691
4	16.433	28612	3390	0.790
Total		3622362	468758	100.000