

Sample Name :RGD

Cat No. : RP20297

Lot No. :E6863426D

Time Processed :23:27:52

Month-Day-Year Processed :04/15/2026

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ21010375

<Chromatogram>

mV

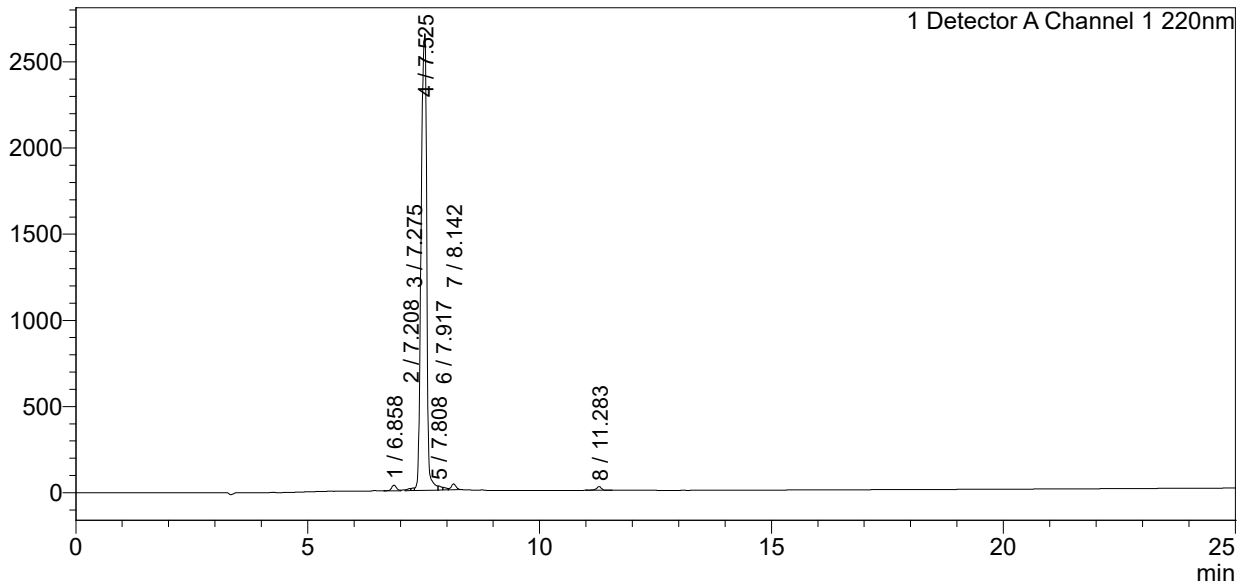

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.858	242229	32555	1.052
2	7.208	69503	12716	0.302
3	7.275	61899	14737	0.269
4	7.525	22046716	2650225	95.714
5	7.808	124986	23822	0.543
6	7.917	77733	14346	0.337
7	8.142	243380	34150	1.057
8	11.283	167497	21751	0.727
Total		23033944	2804301	100.000