

Sample Name:IRBP (1-20), human  
Cat No. : RP20269  
Lot No. : E6889323F  
Time Processed :3:53:39  
Month-Day-Year Processed :06/16/2023

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm

Equipment: GR11010440

### <Chromatogram>

mV

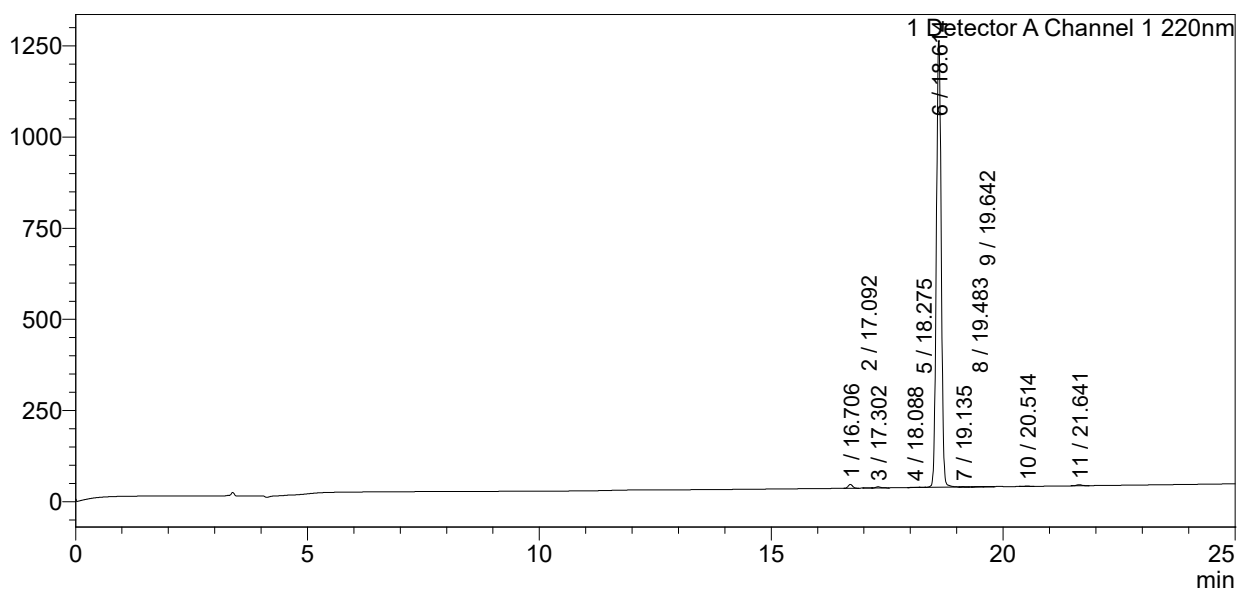

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.706	70180	10734	0.779
2	17.092	1441	224	0.016
3	17.302	22671	3204	0.252
4	18.088	7113	761	0.079
5	18.275	1941	309	0.022
6	18.614	8867843	1226010	98.454
7	19.135	1717	295	0.019
8	19.483	2635	278	0.029
9	19.642	2421	281	0.027
10	20.514	5842	741	0.065
11	21.641	23256	2902	0.258
Total		9007058	1245740	100.000