

Sample Name :IRBP (1-20), human
Cat No. : RP20269
Lot No. : E6909125C
Time Processed :21:08:46
Month-Day-Year Processed :03/17/2025

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm
Equipment: ZJ19010015

<Chromatogram>

mV

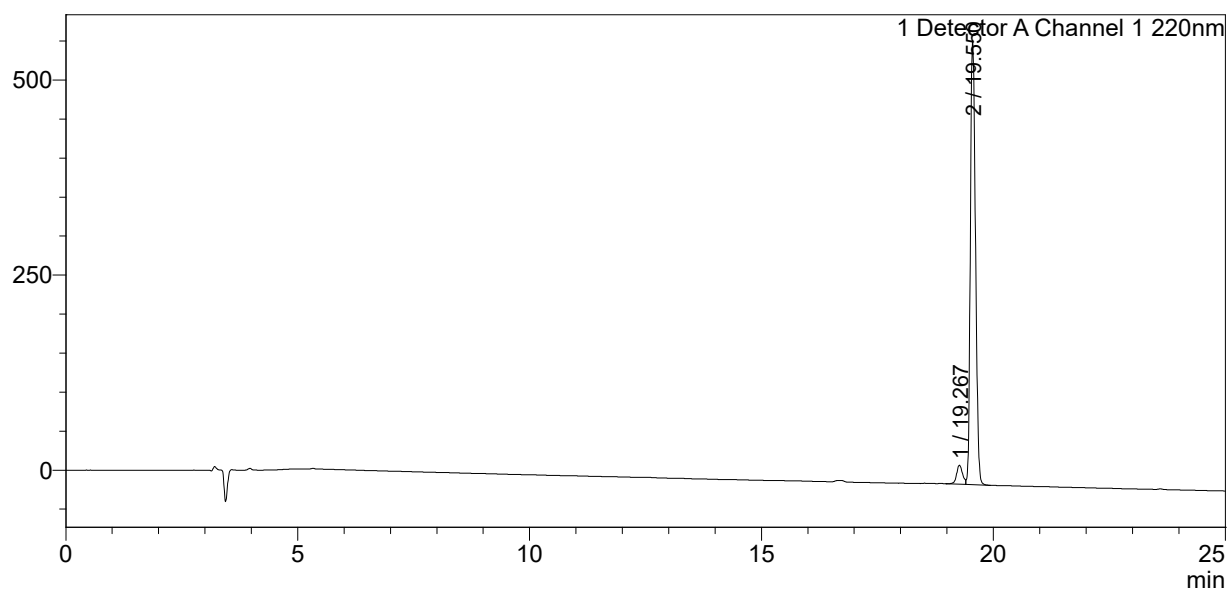

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	19.267	220135	24524	4.811
2	19.550	4355290	569238	95.189
Total		4575426	593761	100.000