

Sample Name :IRBP (1-20), human
Cat No. : RP20269
Lot No. : E6935823F
Time Processed :13:30:39
Month-Day-Year Processed :06/16/2023

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
10.00	Pumps	B.Conc	35
35.00	Pumps	B.Conc	95
37.00	Pumps	B.Conc	95
37.01	Pumps	B.Conc	5
45.00	Pumps	B.Conc	5
45.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm

Equipment: ZJ20010140

<Chromatogram>

mV

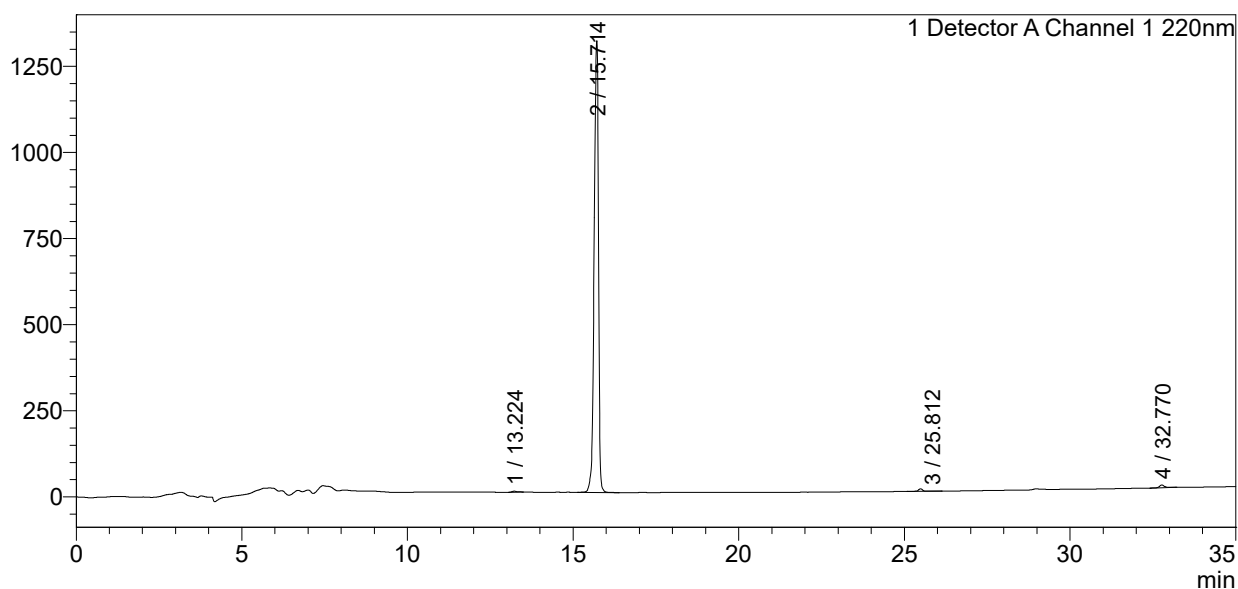

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.224	38303	3105	0.316
2	15.714	11908879	1312254	98.335
3	25.812	71841	579	0.593
4	32.770	91448	8086	0.755
Total		12110471	1324023	100.000