


Mass Spectrum

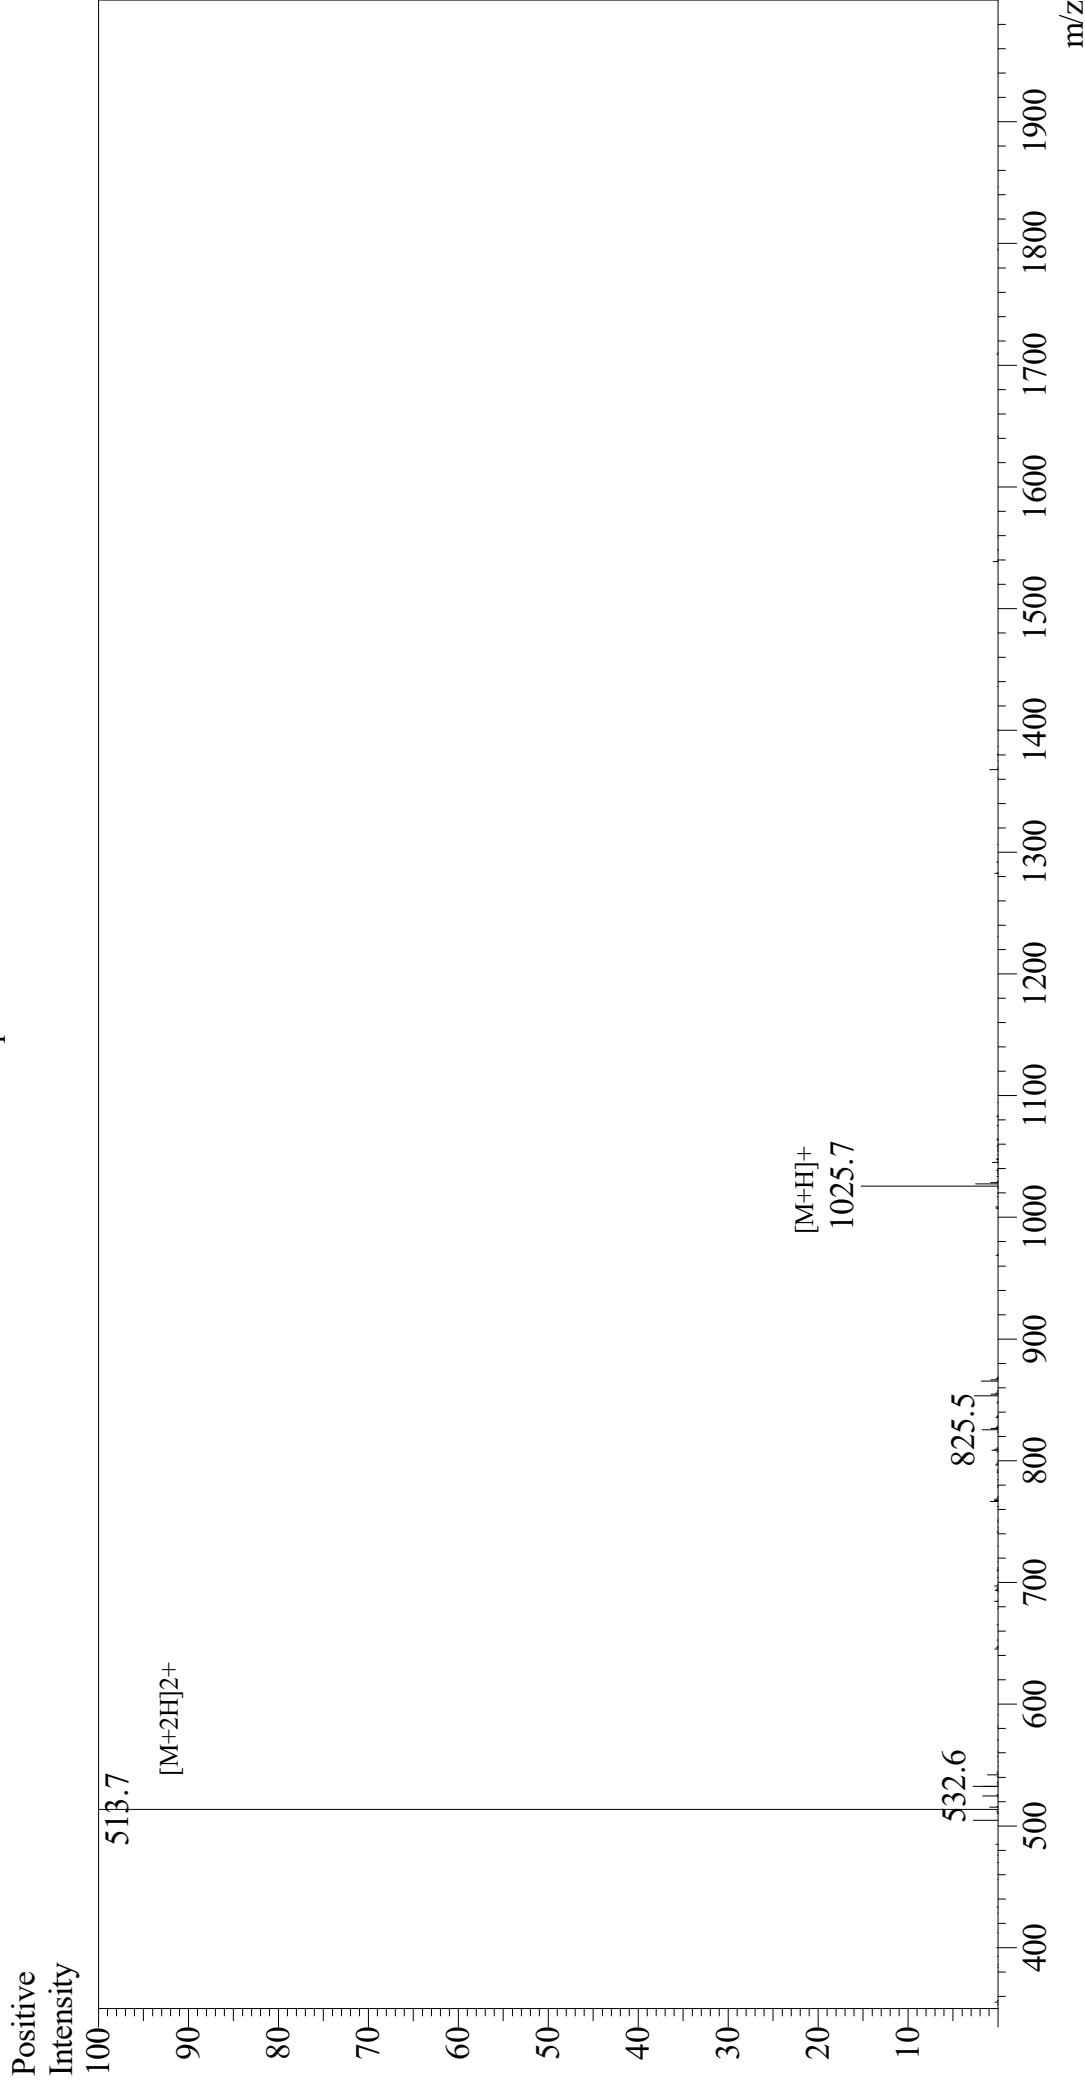

Sample Information
Month-Day Processed : 08/30/22
Time Processed : 11:18:17 AM
Injection Volume : 0.1
Sample Name : RGD
Cat No. : RP20297
Lot No. : E7084722H
Theoretical MW : 1025.06
Observed MW : 1025.4

Interface : ESI
Nebulizing Gas Flow : 1.5 L/min
CDL Temp : 250
Block Temp : 200
Equipment : ZJ22010150
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H₂O / 50% MeOH