


# Mass Spectrum

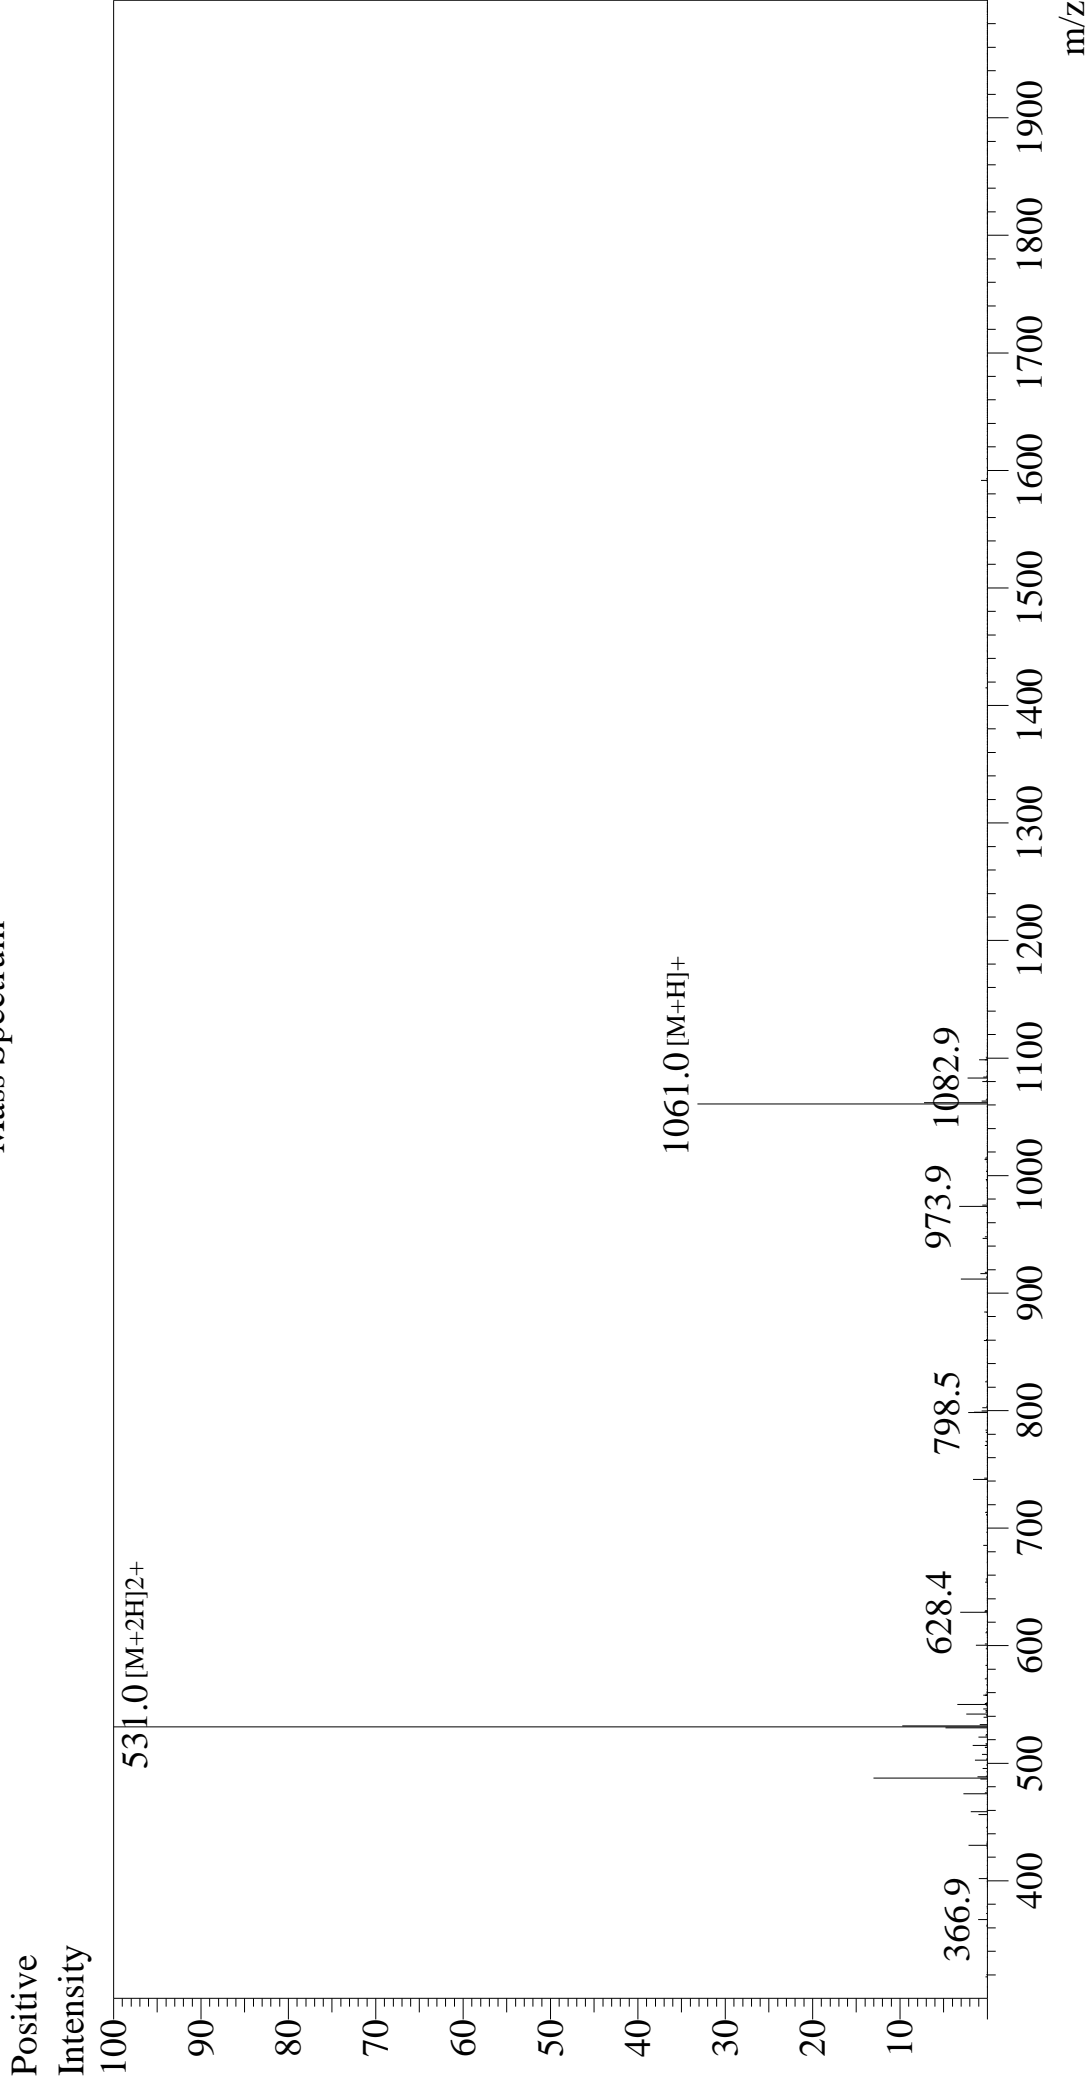

Sample Information		Equipment	
Month-Day Processed :	08/03/24	Interface	:ZJ22010150
Time Processed :	15:57:24	Nebulizing Gas Flow	: +4.5 kV
Injection Volume :	0.2	CDL Temp	:5 L/min
Sample Name :	β-Amyloid (25-35)	Drying Gas Flow	:0.2 ml/min
Cat No. :	RP10008	T.Flow	:50%H2O/50% MeOH
Lot No. :	E7210324H	B.conc	
Theoretical MW :	1060.27		
Observed MW :	1060.0		