

Sample Name: Calcitonin Gene Related Peptide (CGRP), rat  
Cat No. : RP11095  
Lot No. : E7262424D  
Time Processed : 8:03:50 AM  
Month-Day-Year Processed : 05/25/2024


Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
Total Flow: 1 ml/min  
Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>  
<Detector A>  
Column : Inertsil ODS-SP 4.6 x 250 mm  
Equipment: ZJ17010508

<Chromatogram>

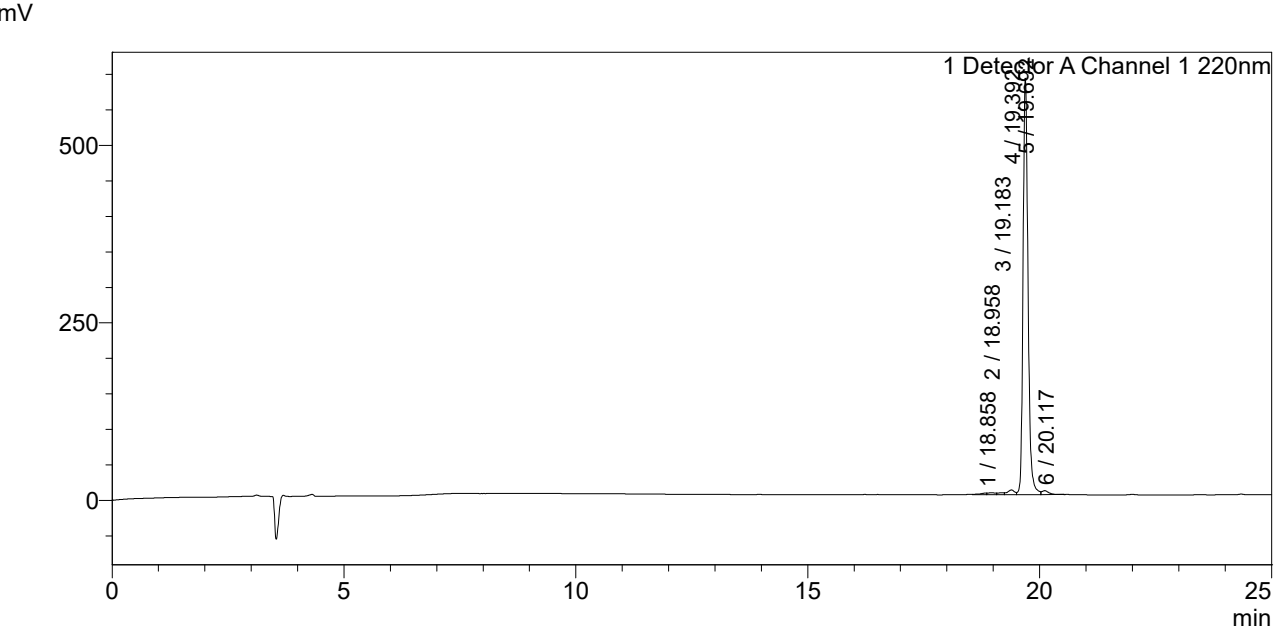

<Peak Table>

Detector A Channel 1 220nm				
Peak#	Ret. Time	Area	Height	Area%
1	18.858	24626	2284	0.537
2	18.958	32887	2781	0.718
3	19.183	25686	2741	0.561
4	19.392	69177	6598	1.510
5	19.692	4370846	586888	95.388
6	20.117	58932	5483	1.286
Total		4582154	606776	100.000