

Sample Name :Substance P  
 Cat No. :RP10178  
 Lot No. :E7401522C  
 Time Processed :13:02:15  
 Month-Day-Year Processed :03/21/2022

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
32.00	Pumps	B.Conc	95
32.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010324

### <Chromatogram>

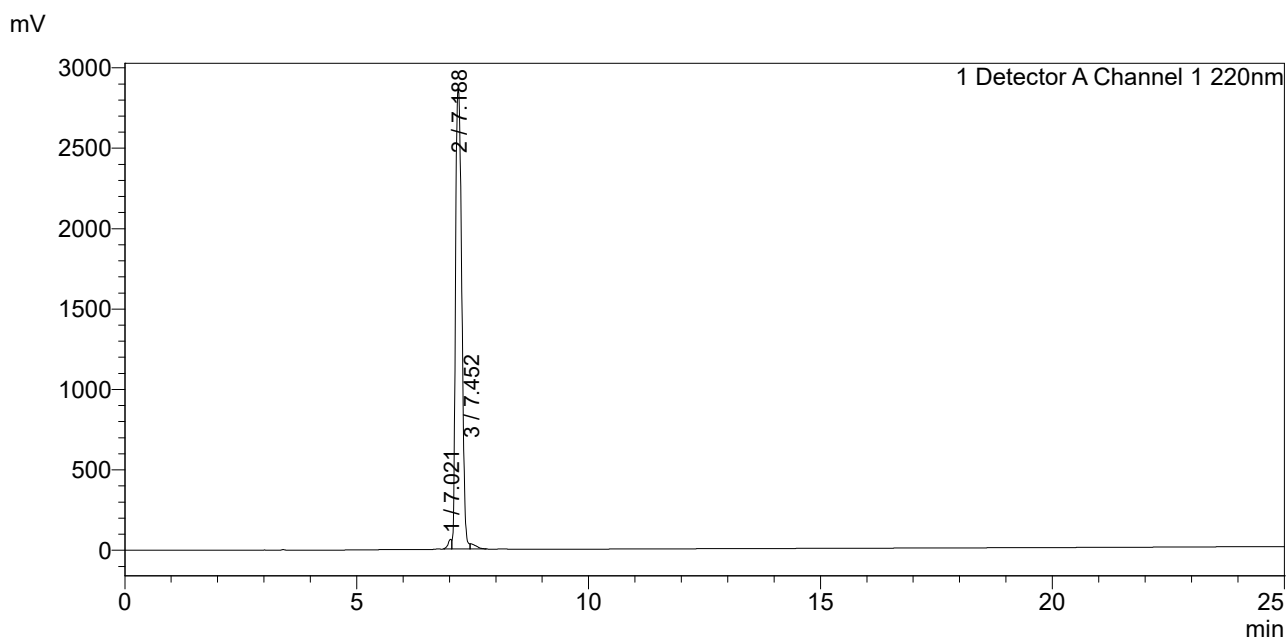

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.021	315738	59634	1.166
2	7.188	26485162	2858896	97.813
3	7.452	276431	32102	1.021
Total		27077331	2950632	100.000