

Sample Name : Calcitonin Gene Related Peptide (CGRP), rat  
 Cat No. : RP11095  
 Lot No. : E7476422G  
 Time Processed : 12:59:06  
 Month-Day-Year Processed : 07/20/2022

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

### <Chromatogram>

mV

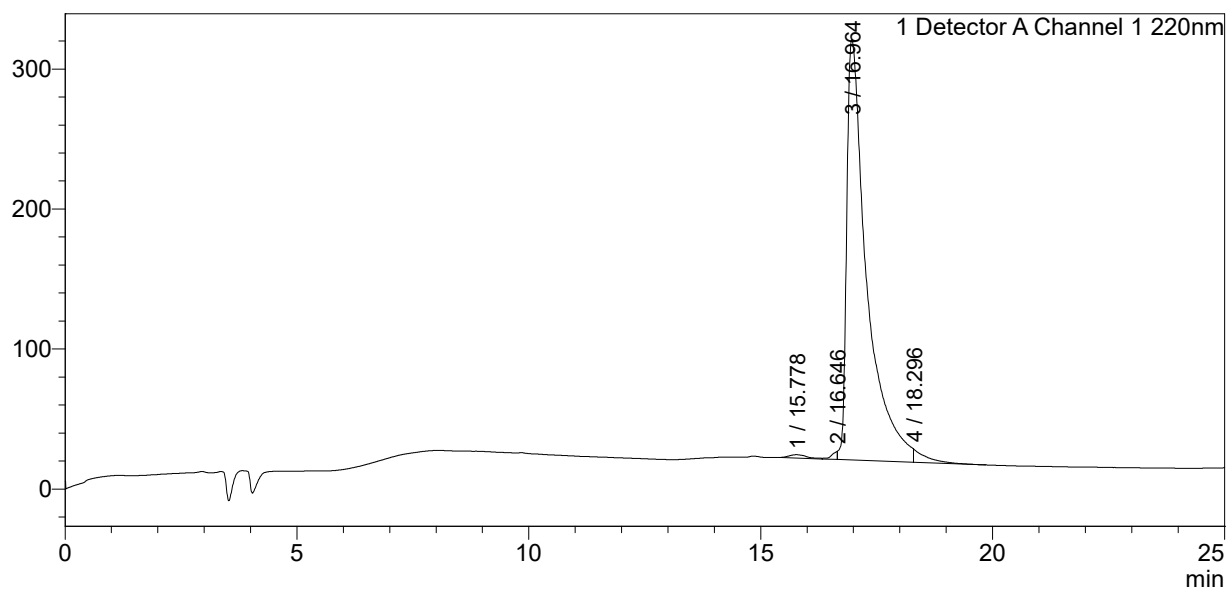

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.778	61352	2317	0.662
2	16.646	46294	5599	0.499
3	16.964	8983356	300344	96.906
4	18.296	179195	9667	1.933
Total		9270197	317926	100.000