


Mass Spectrum

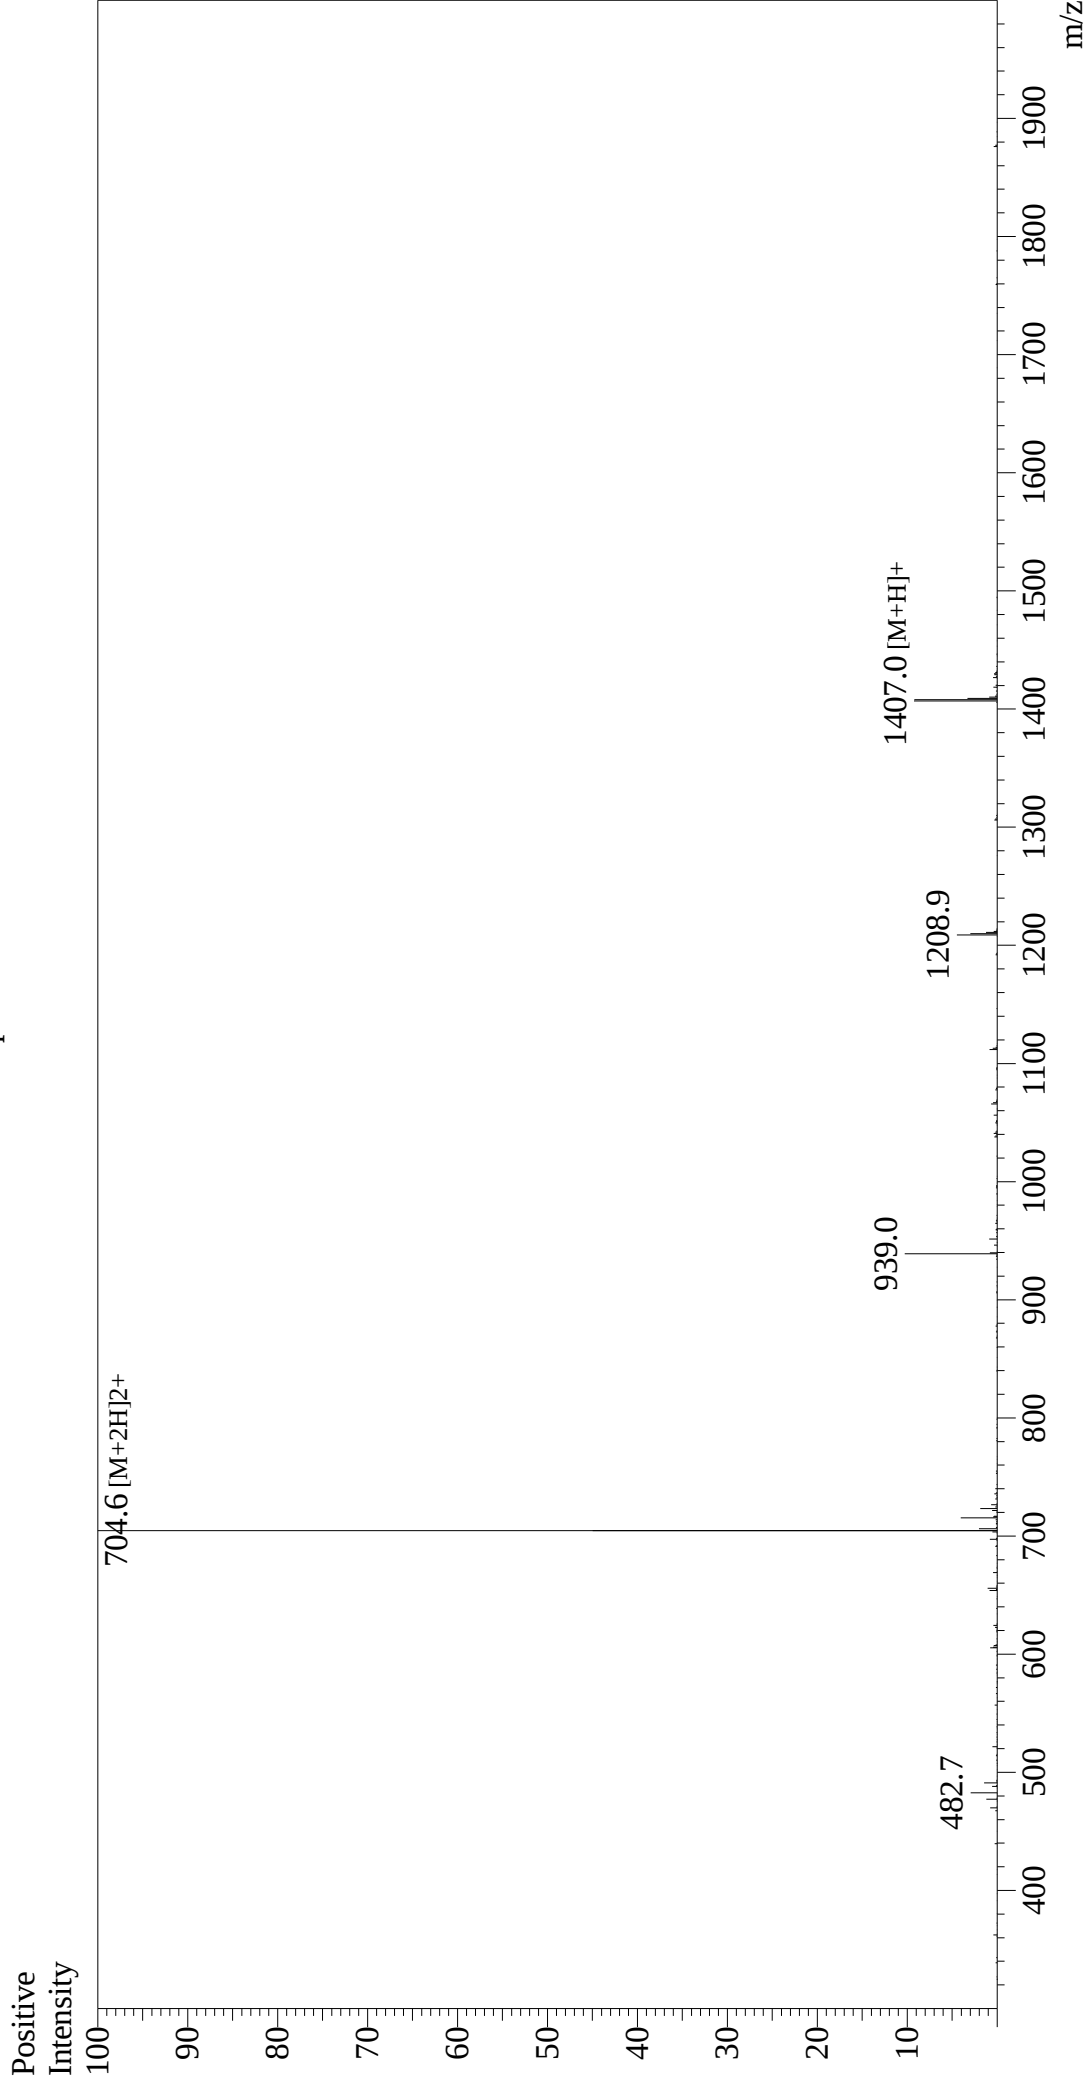

Sample Information

Month-Day Processed :	07/29/22	Equipment	:ZJ22010150
Time Processed :	8:48:42 AM	Interface Bias	: +4.5 kV
Injection Volume :	0.1	Drying Gas Flow	:5 L/min
Sample Name :	Hepatitis B Virus Core (128-140)	T.Flow	:0.2 ml/min
Cat No. :	RP17313	B.conc	:50%H2O/50%MeOH
Lot No. :	E7478722G		
Theoretical MW:1406.63			
Observed MW :1407.2			