

Sample Name:IRBP (1-20), human
 Cat No. : RP20269
 Lot No. : E7480522G
 Time Processed :1:21:02 AM
 Month-Day-Year Processed :07/23/2022

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010140

<Chromatogram>

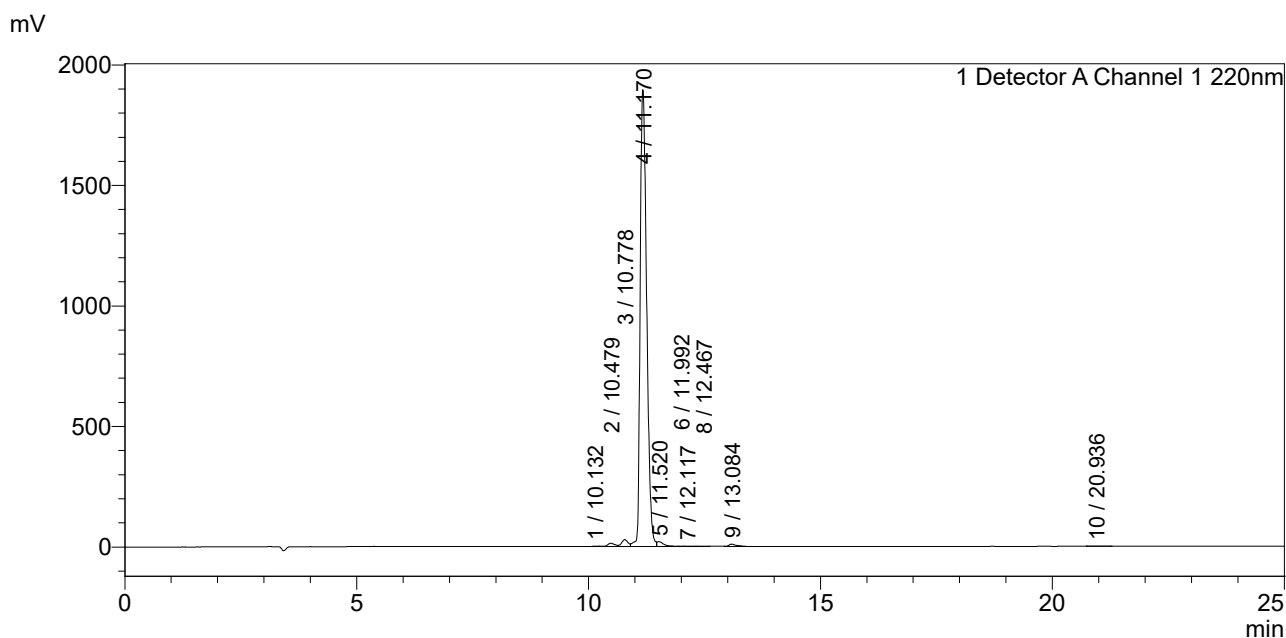

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.132	10905	1232	0.057
2	10.479	147354	13419	0.770
3	10.778	272139	28653	1.423
4	11.170	18306874	1895823	95.708
5	11.520	212361	19740	1.110
6	11.992	10244	1510	0.054
7	12.117	15892	1406	0.083
8	12.467	16843	1240	0.088
9	13.084	118371	9878	0.619
10	20.936	16880	778	0.088
Total		19127864	1973678	100.000