


Mass Spectrum

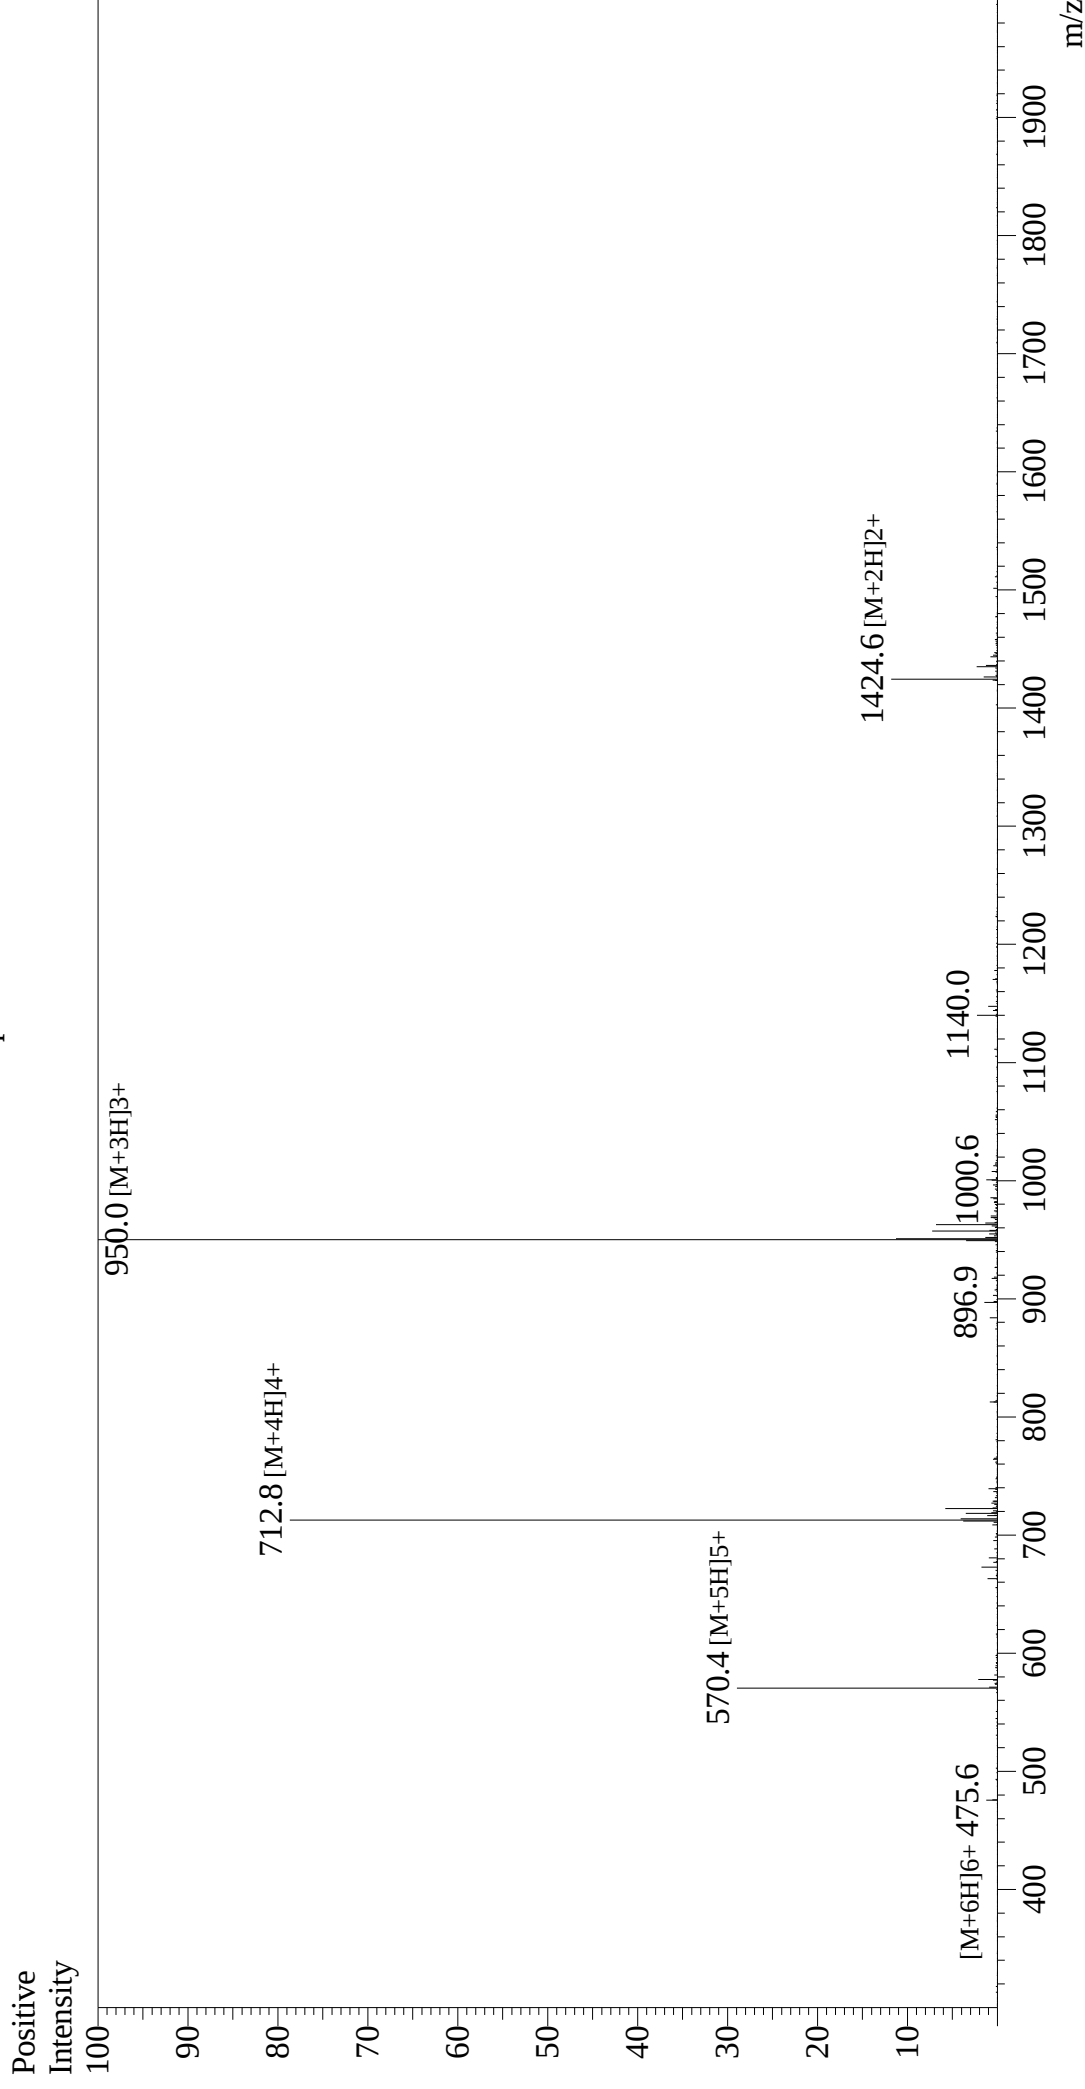

Sample Information

Month-Day Processed : 06/24/25
 Time Processed : 23:08:49
 Injection Volume : 0.2
 Sample Name : Melittin, honey bee
 Cat No. : RP20415
 Lot No. : E7516025F
 Theoretical MW: 2847.50
 Observed MW : 2847.0

Interface

Interface : ESI
 Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200

Equipment

Equipment : ZJ21010035
 Interface Bias : +4.5 kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2 ml/min
 B.conc : 50% H₂O/50% MeOH