


Mass Spectrum

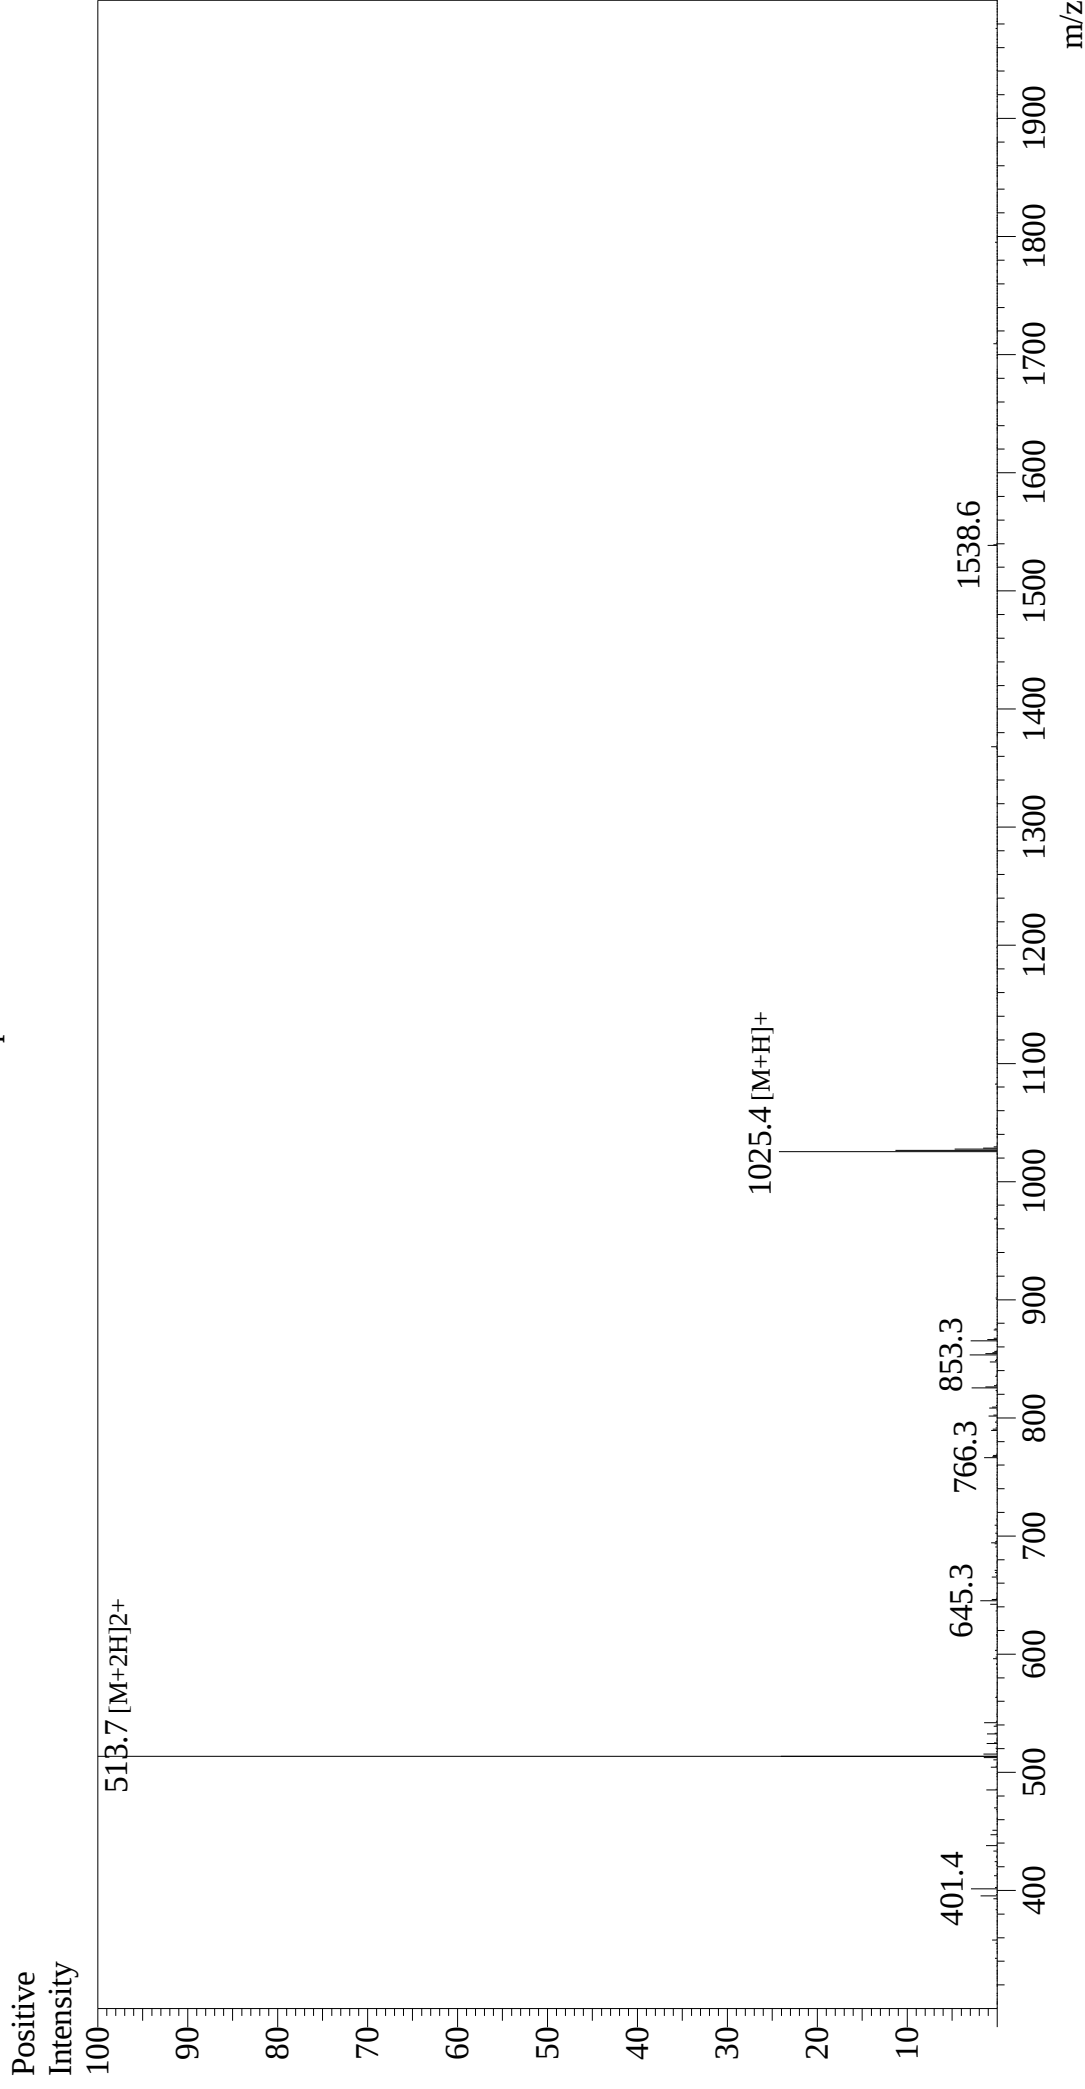

Sample Information

Month-Day Processed : 07/31/25
Time Processed : 17:43:29
Injection Volume : 0.3
Sample Name : RGD

Cat No. : RP20297
Lot No. : E7533625G
Theoretical MW : 1025.06
Observed MW : 1025.4

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : ZJ22010150
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H₂O/50%MeOH