

Sample Name :Substance P
 Cat No. : RP10178
 Lot No. : E7558825A
 Time Processed :15:30:01
 Month-Day-Year Processed :01/21/2025
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm
 Equipment: ZJ21010376

<Chromatogram>

mV

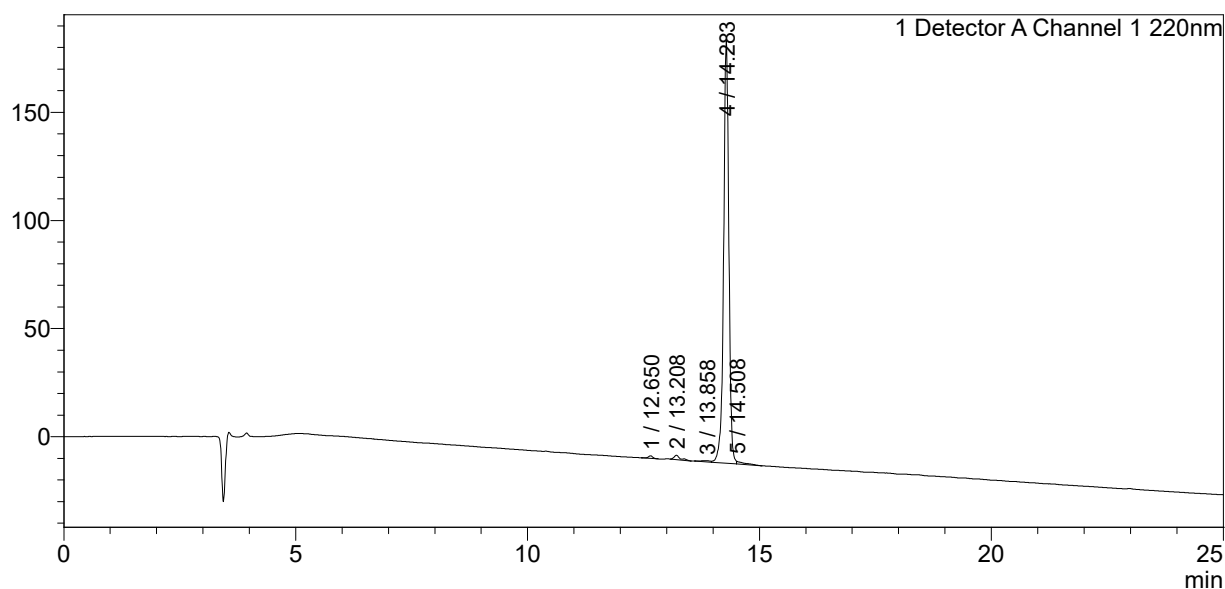

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.650	8171	1208	0.516
2	13.208	18308	1990	1.157
3	13.858	8297	625	0.524
4	14.283	1532407	195490	96.815
5	14.508	15641	1302	0.988
Total		1582823	200615	100.000