

Sample Name : Calcitonin Gene Related Peptide (CGRP), rat
Cat No. : RP11095
Lot No. : E7618022J

Time Processed : 4:37:28 PM

Month-Day-Year Processed : 11/04/2022

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow: 1 ml/min

Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column : Inertsil ODS-SP 4.6 x 250 mm

Equipment: GR11010440

<Chromatogram>

mV

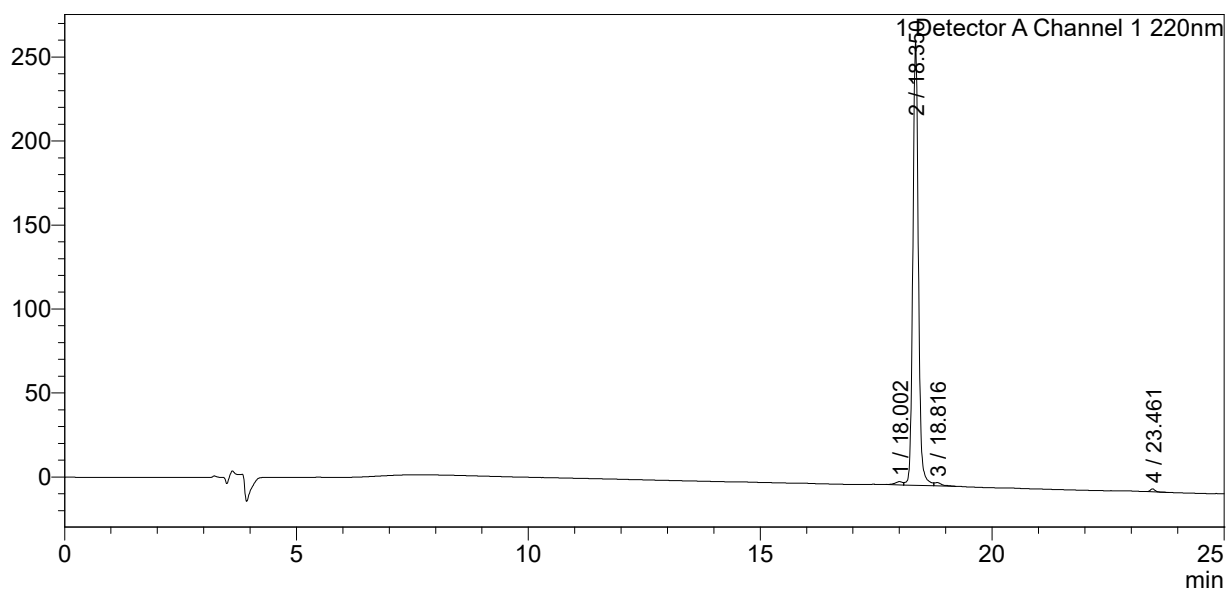

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	18.002	21804	1953	0.964
2	18.350	2204984	264921	97.517
3	18.816	21173	1914	0.936
4	23.461	13167	1830	0.582
Total		2261127	270619	100.000