

Sample Name :Biotin-β-Amyloid (1-40)

Cat No. : RP30249

Lot No. : E7671526A

Time Processed :20:45:50

Month-Day-Year Processed :01/21/2026

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :UniPSN 30-300 30um, 4.6x250mm

<Chromatogram>

mV

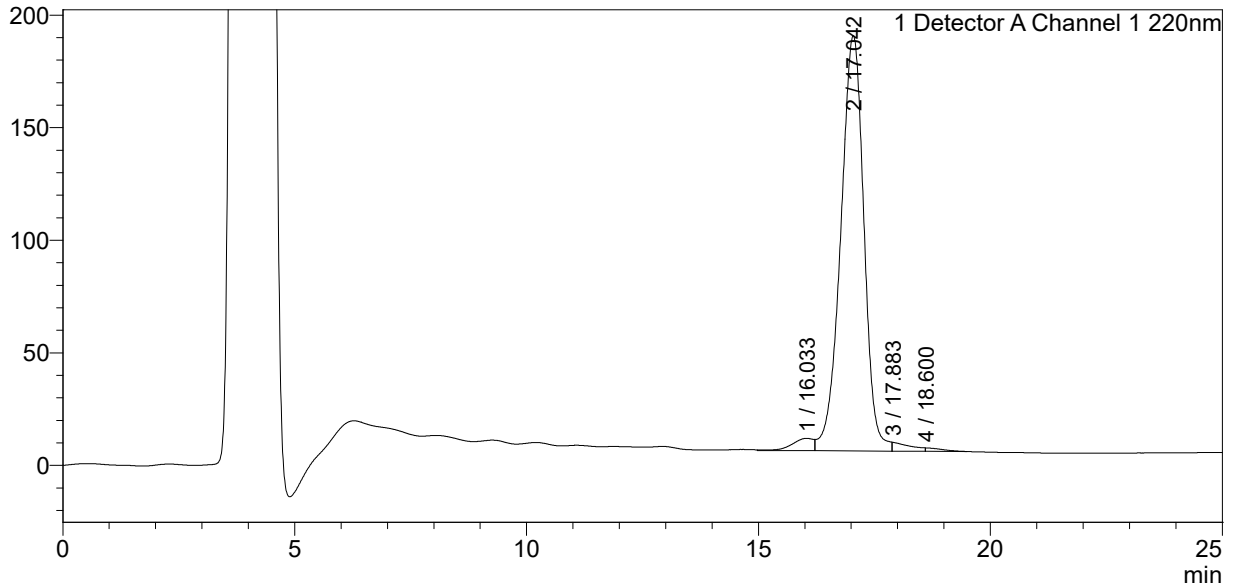

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.033	175523	5505	2.604
2	17.042	6420427	184472	95.260
3	17.883	107333	3973	1.593
4	18.600	36592	1506	0.543
Total		6739875	195455	100.000