

Sample Name :Substance P

Cat No. : RP10178

Lot No. : E7868124C

Time Processed :0:26:41

Month-Day-Year Processed :03/09/2024

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ19010325

### <Chromatogram>

mV

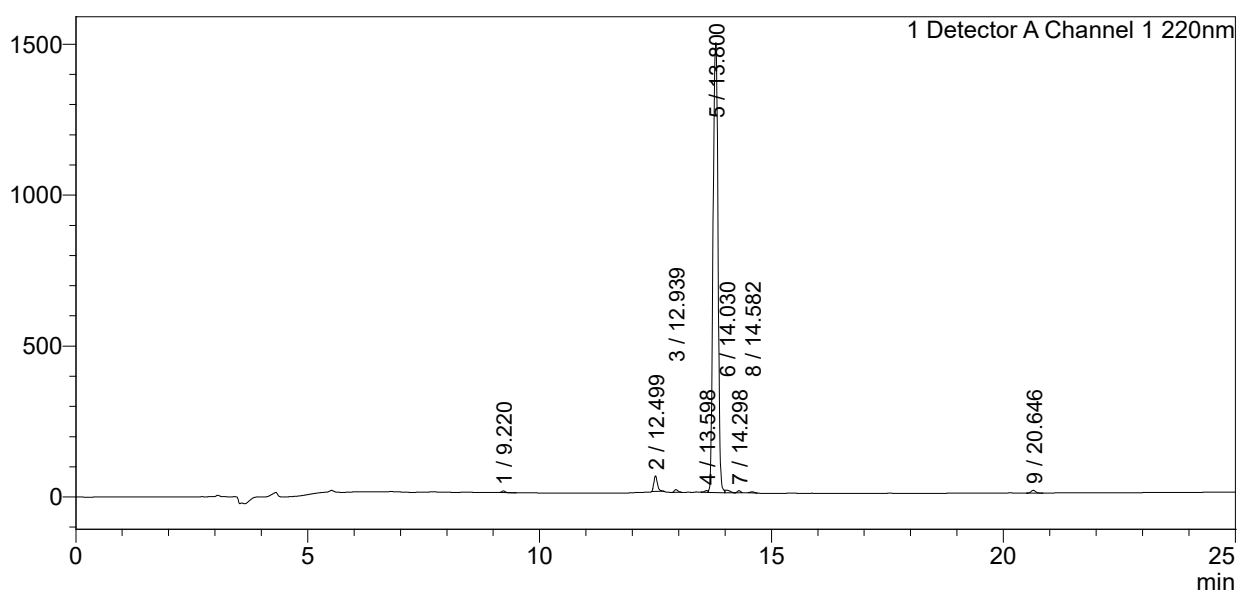

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.220	33530	6011	0.290
2	12.499	275288	51963	2.385
3	12.939	47687	9250	0.413
4	13.598	28700	5568	0.249
5	13.800	10985311	1490741	95.154
6	14.030	59791	8480	0.518
7	14.298	35696	7408	0.309
8	14.582	22487	3865	0.195
9	20.646	56333	9059	0.488
Total		11544823	1592345	100.000