

Sample Name :IRBP (1-20), human
Cat No. : RP20269
Lot No. : E7869524C
Time Processed :20:09:02
Month-Day-Year Processed :03/14/2024

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm
<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm
Equipment: SS-CM-0309

<Chromatogram>

mV

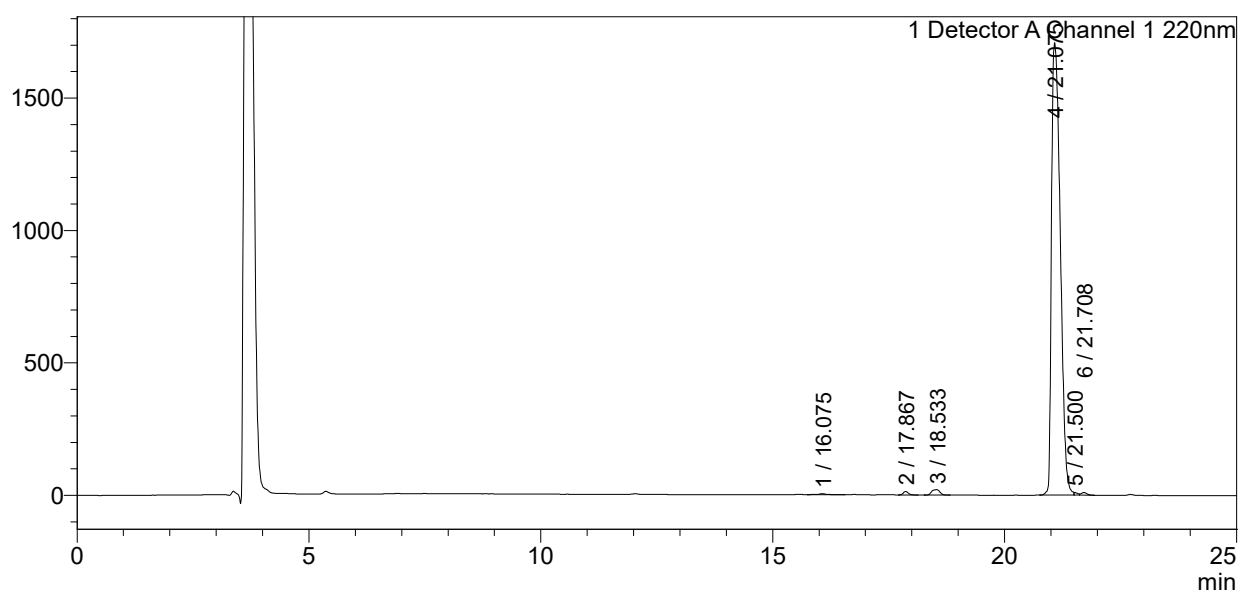

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.075	49865	4076	0.217
2	17.867	97553	12838	0.425
3	18.533	247061	20493	1.076
4	21.075	22420191	1708741	97.688
5	21.500	50647	10621	0.221
6	21.708	85572	9784	0.373
Total		22950889	1766553	100.000