

Sample Name :Biotin-β-Amyloid (1-40)
 Cat No. : RP30249
 Lot No. : E7918025G
 Time Processed :15:20:15
 Month-Day-Year Processed :07/25/2025

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :UniPSN 30-300 30um,4.6x250mm

<Chromatogram>

mV

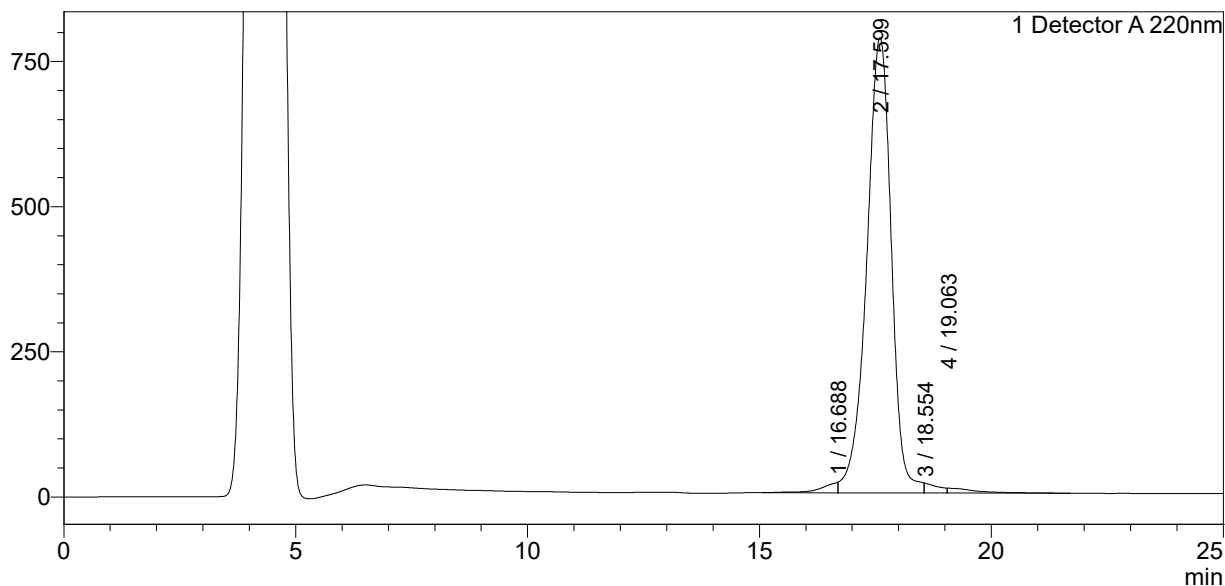

<Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.688	443289	18249	1.473
2	17.599	28916043	784211	96.112
3	18.554	360274	17334	1.197
4	19.063	366274	8396	1.217
Total		30085879	828190	100.000