


Mass Spectrum

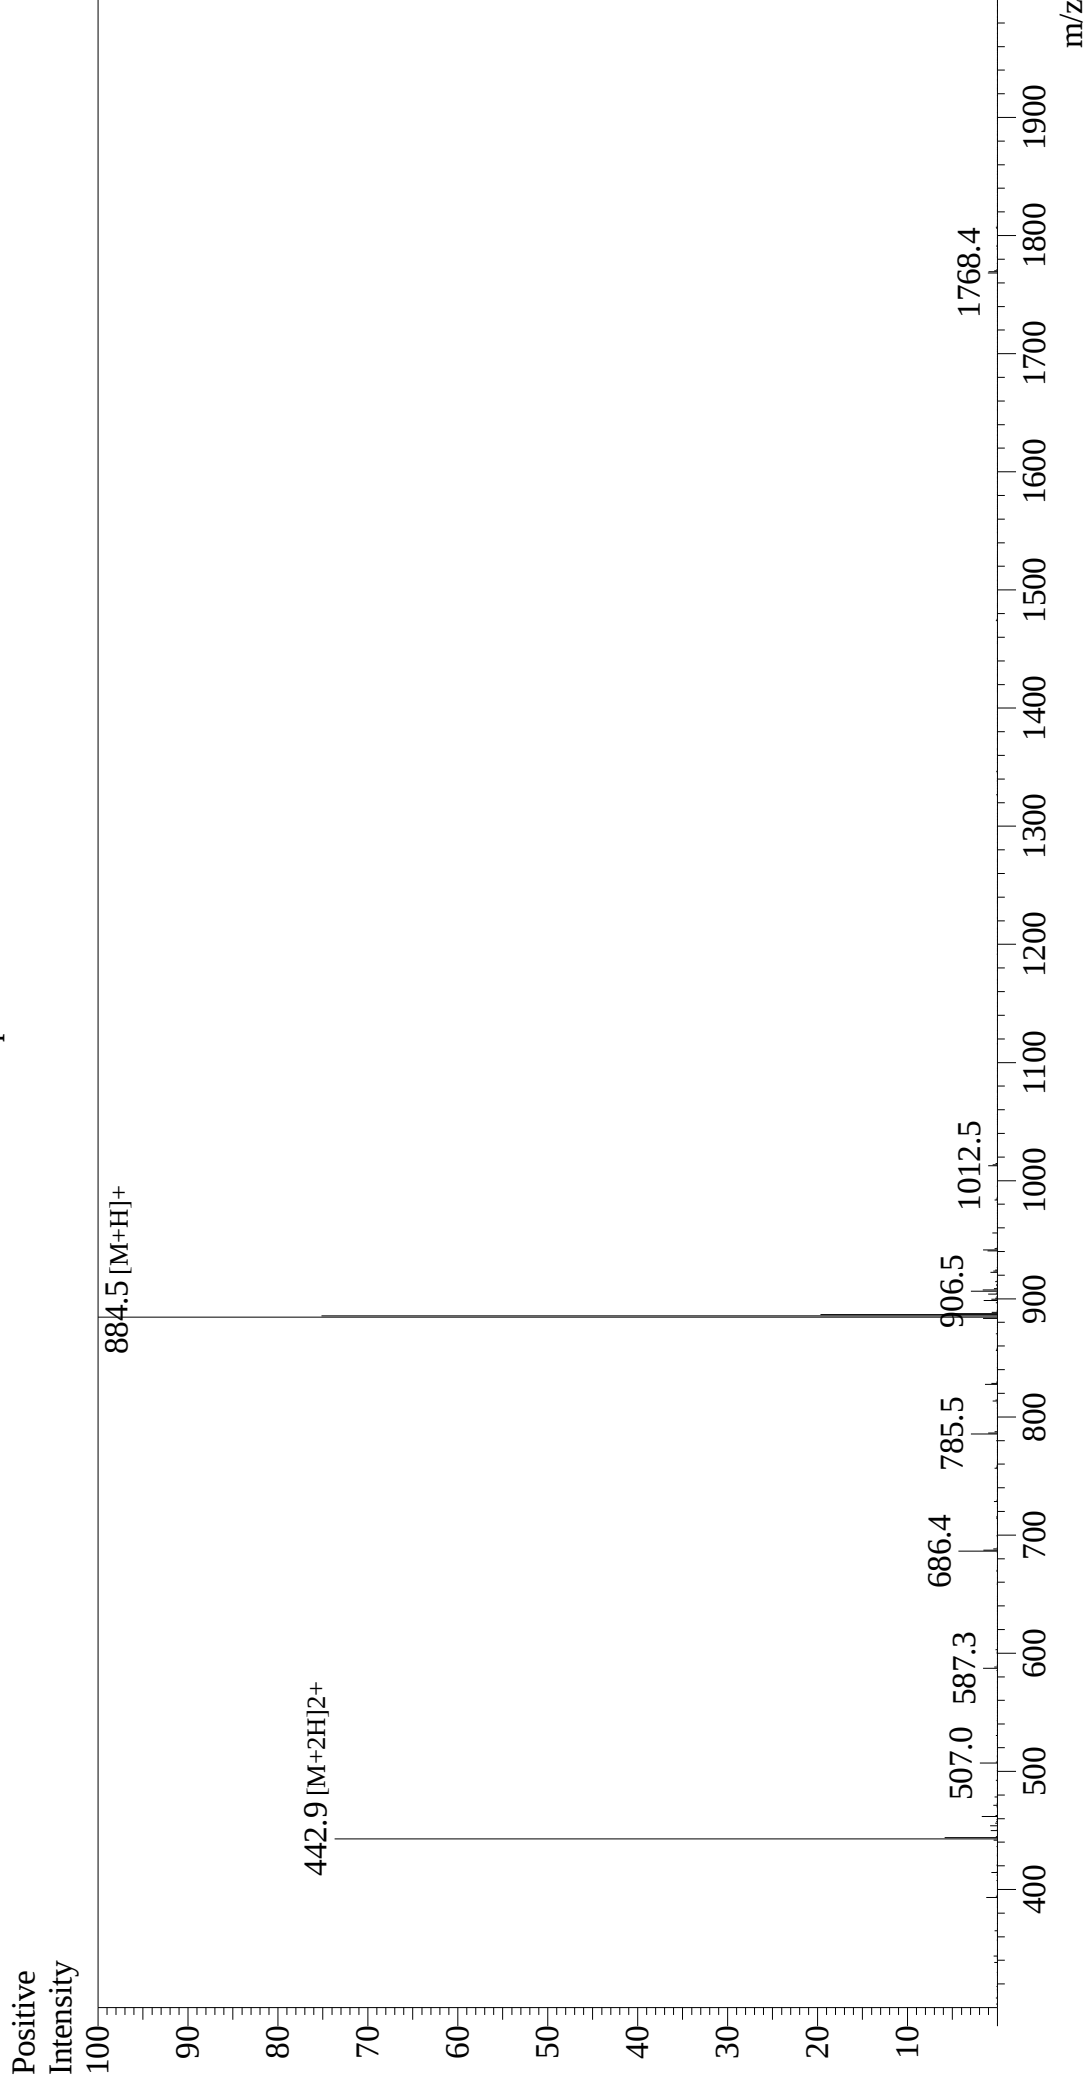

Sample Information

Month-Day Processed : 07/25/25
Time Processed : 19:44:57
Injection Volume : 0.3
Sample Name : KRAS G12V Peptide (VVVGAVGVGK)
Cat No. : RP30229
Lot No. : E7930425G
Theoretical MW: 884.08
Observed MW : 883.5

Interface

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment

Equipment : ZJ21010035
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H₂O/50%MeOH