


Mass Spectrum

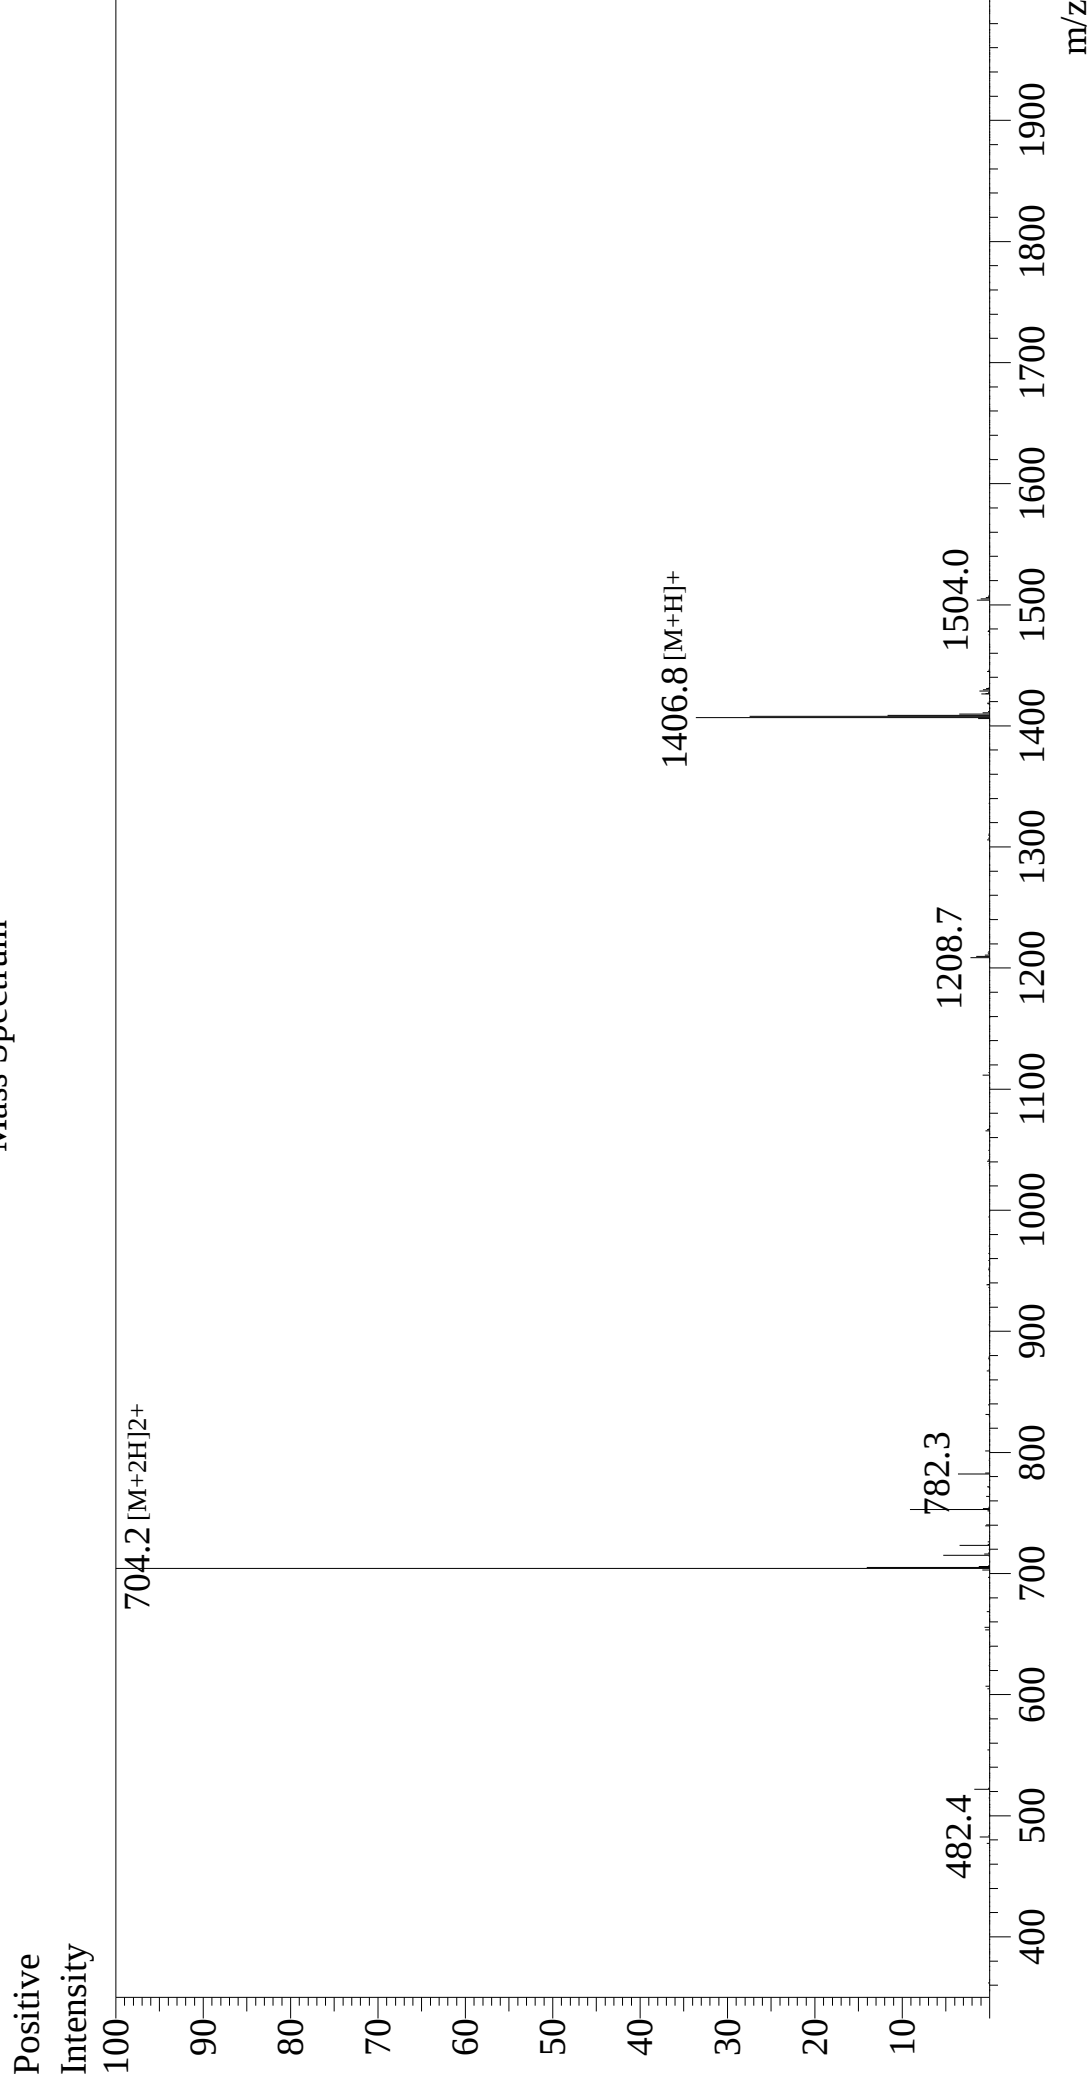

Sample Information

Month-Day Processed : 07/23/25
Time Processed : 21:10:09
Injection Volume : 0.2
Sample Name : Hepatitis B Virus Core (128-140)
Cat No. : RP17313
Lot No. : E7936325G
Theoretical MW: 1406.63
Observed MW : 1406.4

Equipment : ZJ21010035
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200