


Mass Spectrum

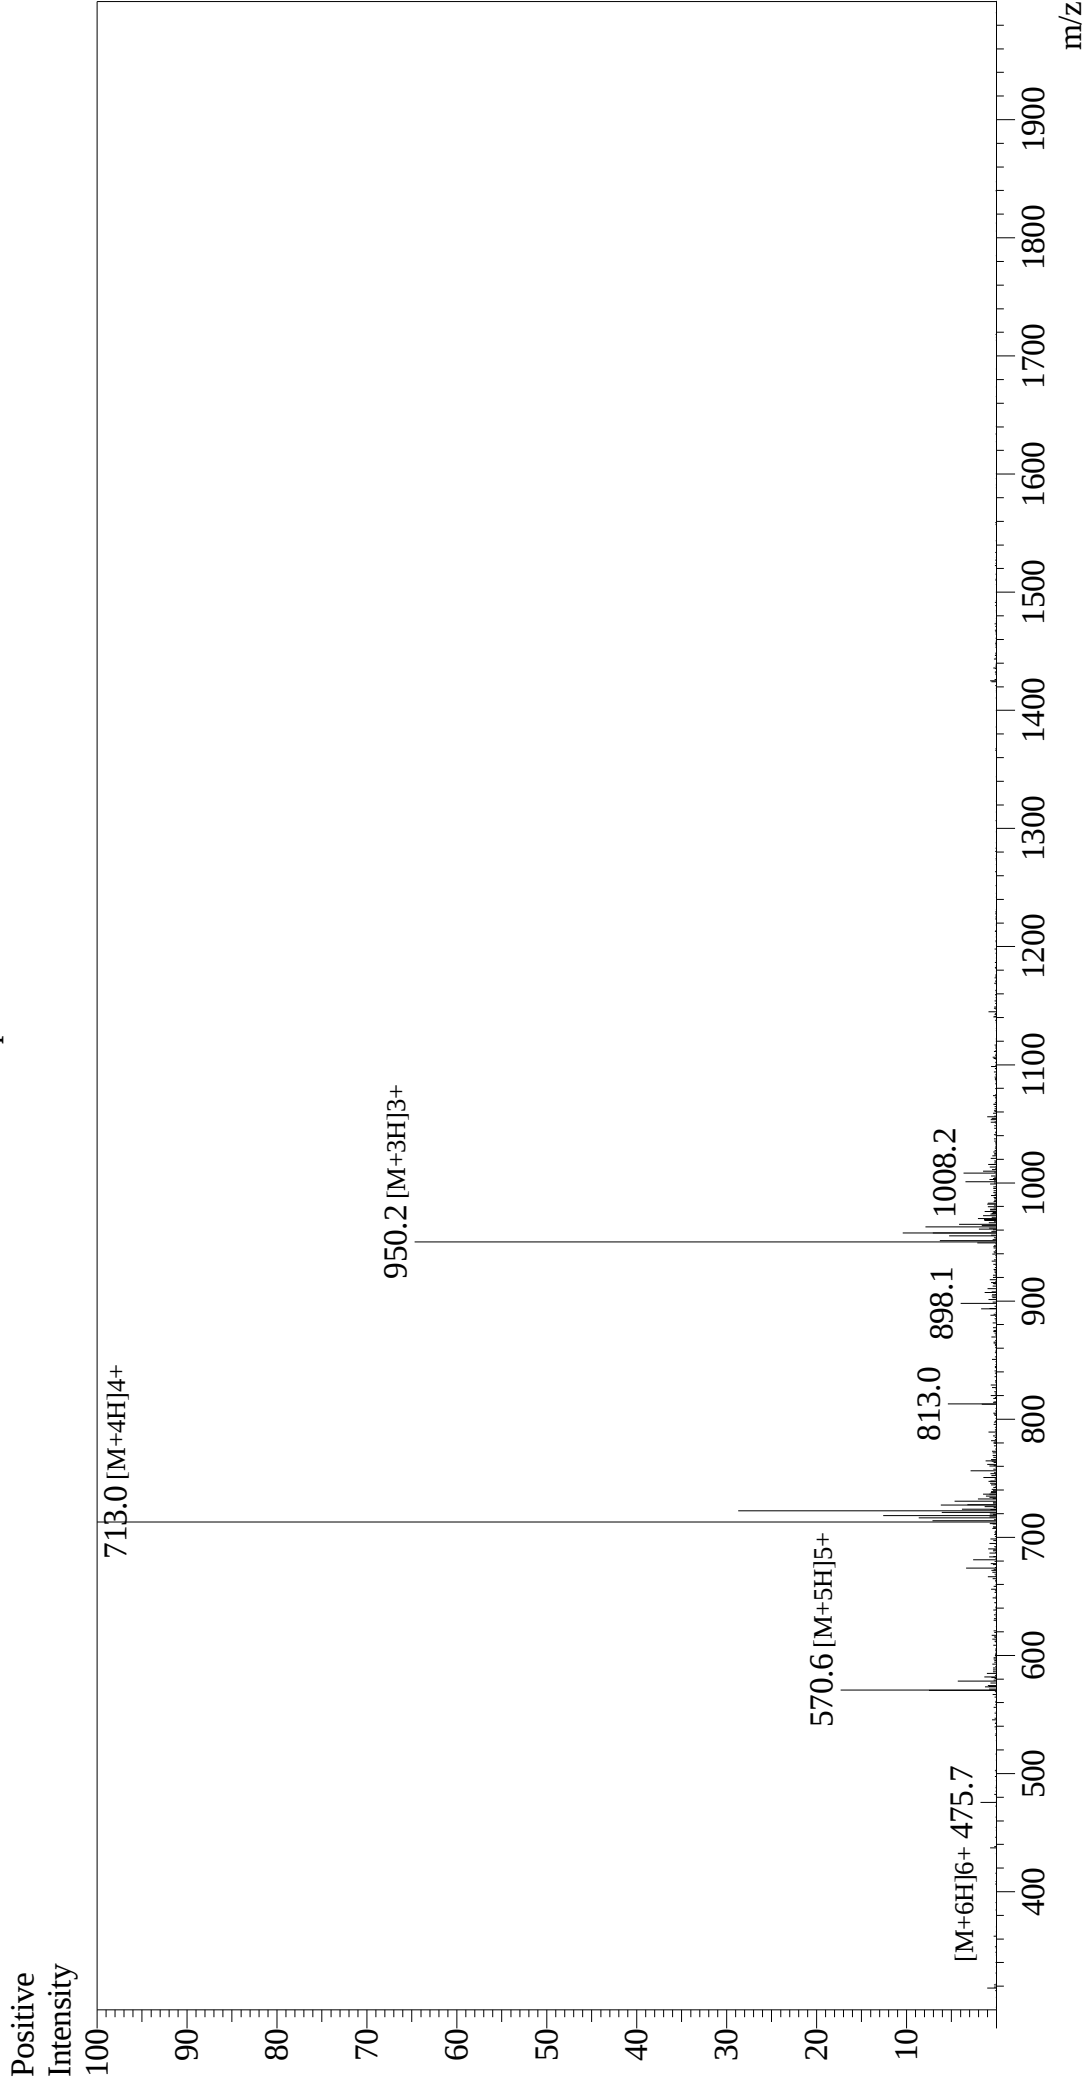

Sample Information

Month-Day Processed : 04/24/23
Time Processed : 22:33:10
Injection Volume : 0.3
Sample Name : Melittin, honey bee
Cat No. : RP20415
Lot No. : E8006423D
Theoretical MW: 2847.50
Observed MW : 2848.0

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : ZJ21010035
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H₂O/50% MeOH