

Sample Name :Substance P
Cat No. : RP10178
Lot No. : E8046723H
Time Processed :3:39:27
Month-Day-Year Processed :08/08/2023

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm
Equipment: ZJ19010324

<Chromatogram>

mV

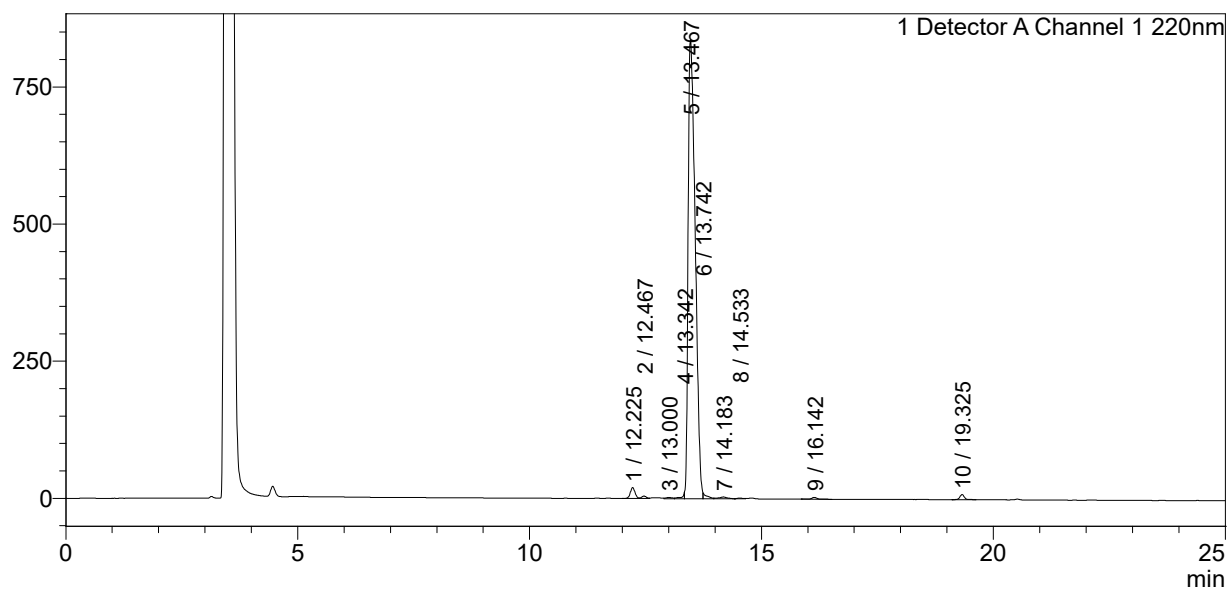

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.225	143623	19865	1.535
2	12.467	33380	4663	0.357
3	13.000	21120	2142	0.226
4	13.342	39459	12141	0.422
5	13.467	8908737	837195	95.238
6	13.742	58326	10679	0.624
7	14.183	45896	3391	0.491
8	14.533	14075	1684	0.150
9	16.142	27876	3392	0.298
10	19.325	61684	9256	0.659
Total		9354176	904407	100.000