

Sample Name : Calcitonin Gene Related Peptide (CGRP), rat
Cat No. : RP11095
Lot No. : E8134723I
Time Processed :18:51:04
Month-Day-Year Processed :09/23/2023

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm

Equipment: SS-CM-0286

<Chromatogram>

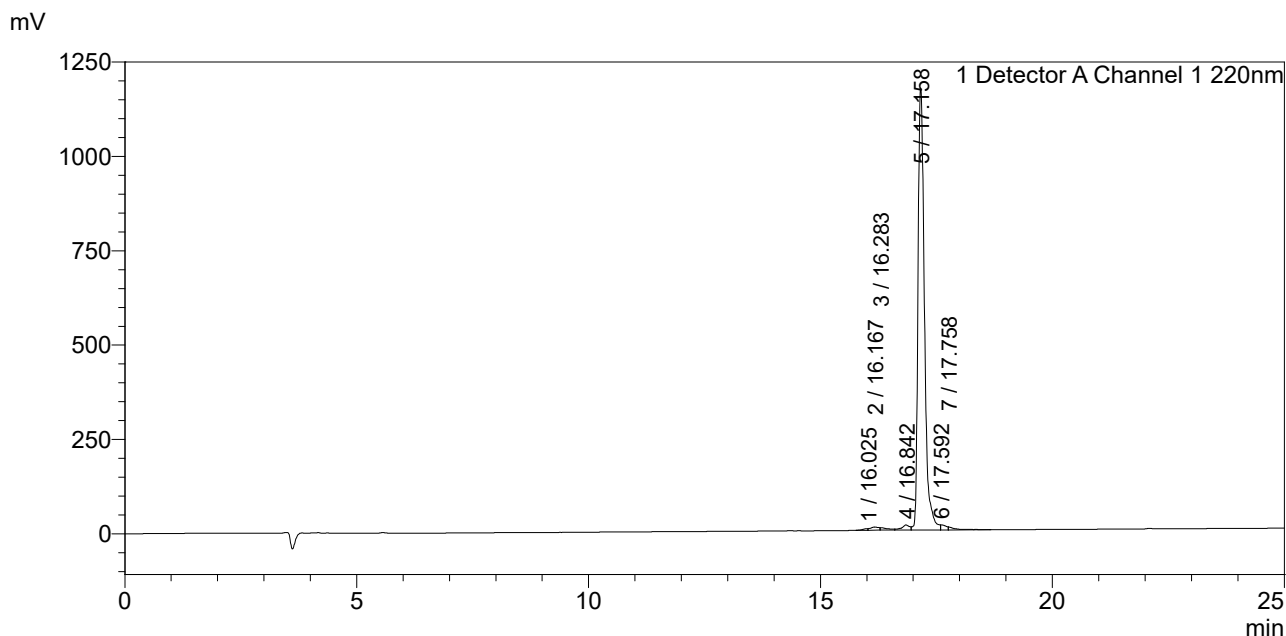

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.025	30387	4287	0.256
2	16.167	104739	8547	0.882
3	16.283	79451	6736	0.669
4	16.842	160862	13506	1.355
5	17.158	11303739	1171093	95.207
6	17.592	110570	13350	0.931
7	17.758	83015	7742	0.699
Total		11872763	1225262	100.000