

Sample Name :MDYKDHDGDYKDHDIDYKDDDDK peptide
 Cat No. :RP21087
 Lot No. :E8203522A
 Time Processed :11:09:57 PM
 Month-Day-Year Processed :01/18/2022

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010011

<Chromatogram>

mV

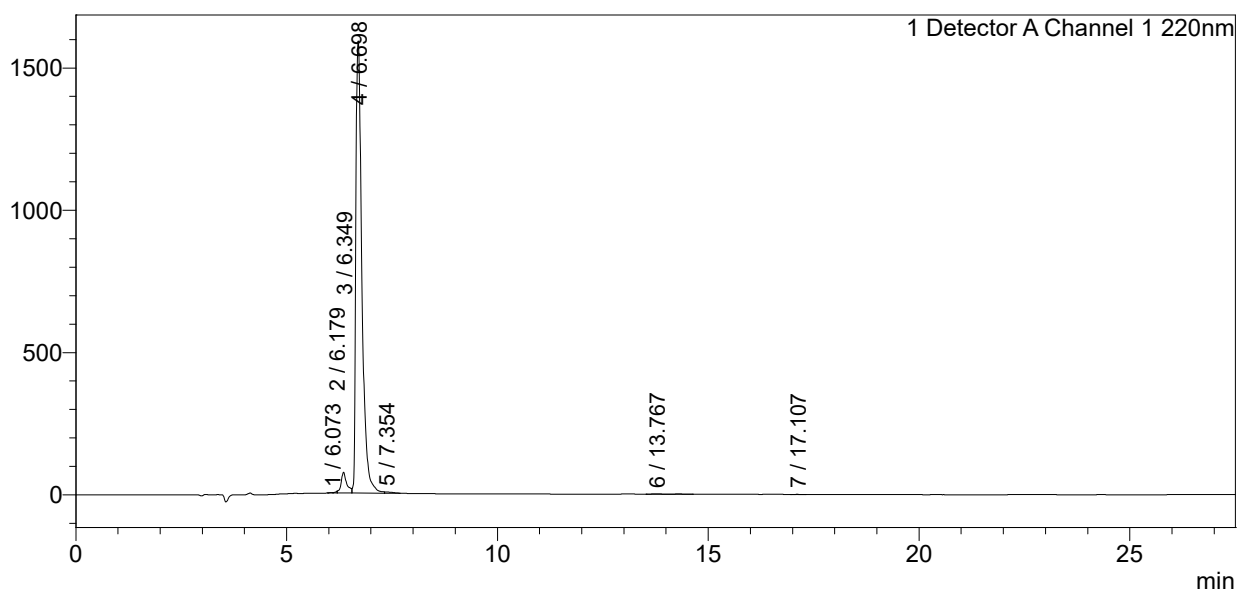

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.073	9681	1715	0.058
2	6.179	22534	4366	0.136
3	6.349	689589	72189	4.149
4	6.698	15832342	1581030	95.250
5	7.354	47661	4242	0.287
6	13.767	16194	494	0.097
7	17.107	3916	396	0.024
Total		16621916	1664434	100.000