


Mass Spectrum

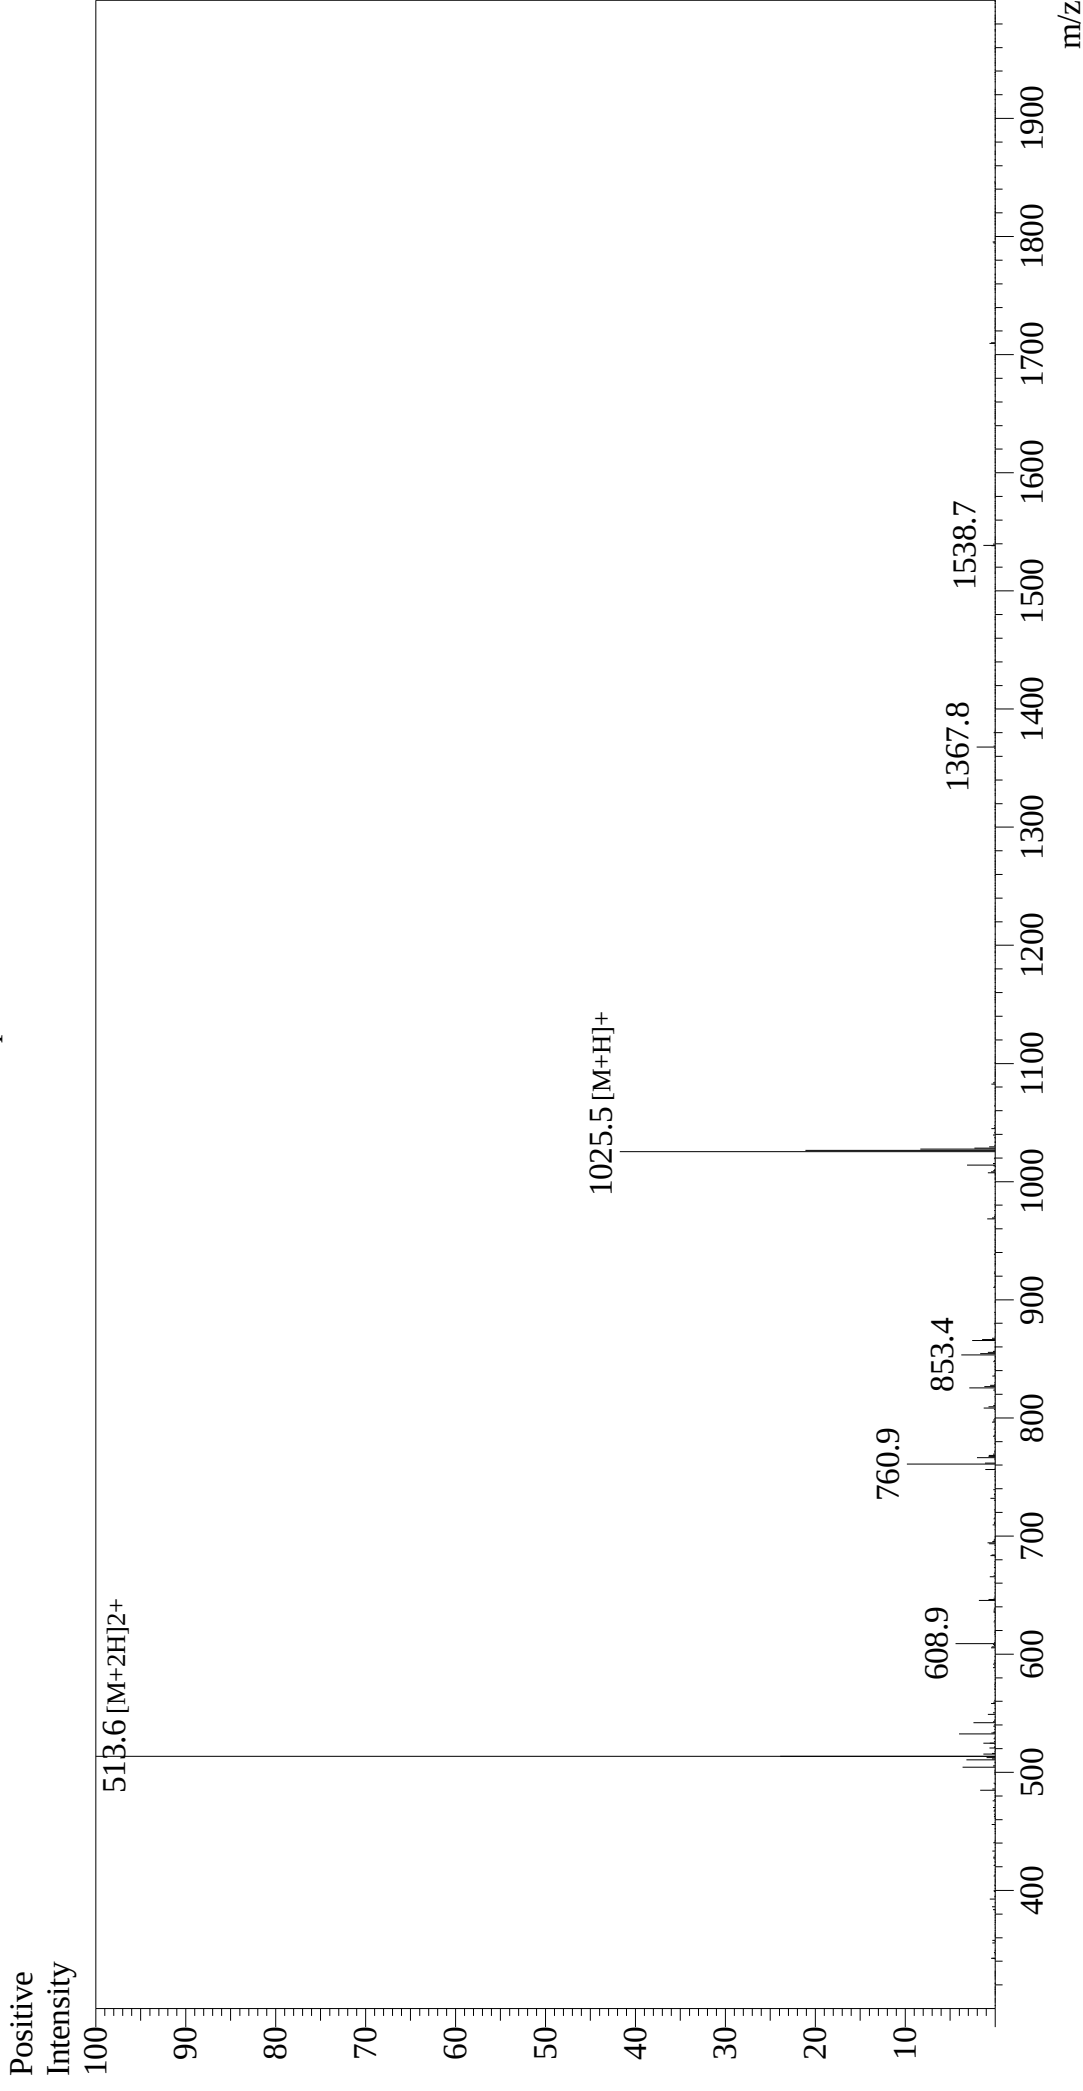

Sample Information

Month-Day Processed : 12/01/25
 Time Processed : 19:42:26
 Injection Volume : 0.2
 Sample Name : RGD
 Cat No. : RP20297
 Lot No. : E8511125K

Theoretical MW: 1025.06

Observed MW: 1025.2

Interface : ESI
 Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200

Equipment : ZJ22010150
 Interface Bias : +4.5 kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2 ml/min
 B.conc : 50% H₂O/50% MeOH