

Sample Name :Substance P
Cat No.: RP10178
Lot No.: E8748722B
Time Processed :20:56:49
Month-Day-Year Processed :02/28/2022

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
Equipment:ZJ19010014

<Chromatogram>

mV

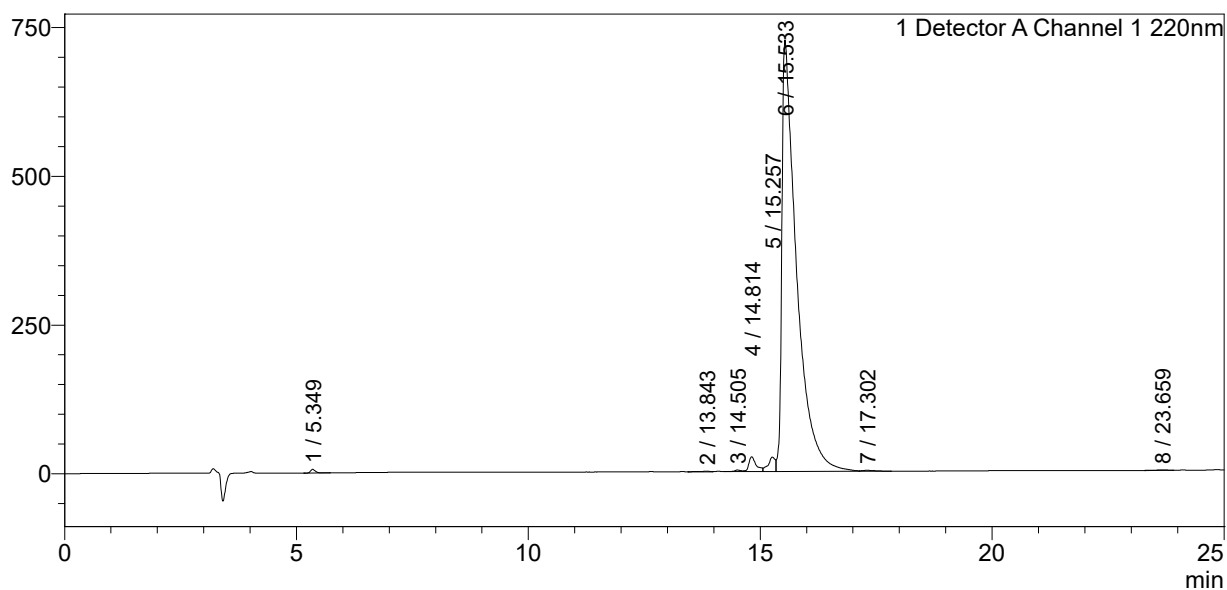

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.349	44974	6232	0.271
2	13.843	14278	888	0.086
3	14.505	31285	2736	0.188
4	14.814	276981	25008	1.669
5	15.257	262073	24254	1.579
6	15.533	15924452	725598	95.945
7	17.302	29086	1482	0.175
8	23.659	14288	823	0.086
Total		16597417	787020	100.000