


Mass Spectrum

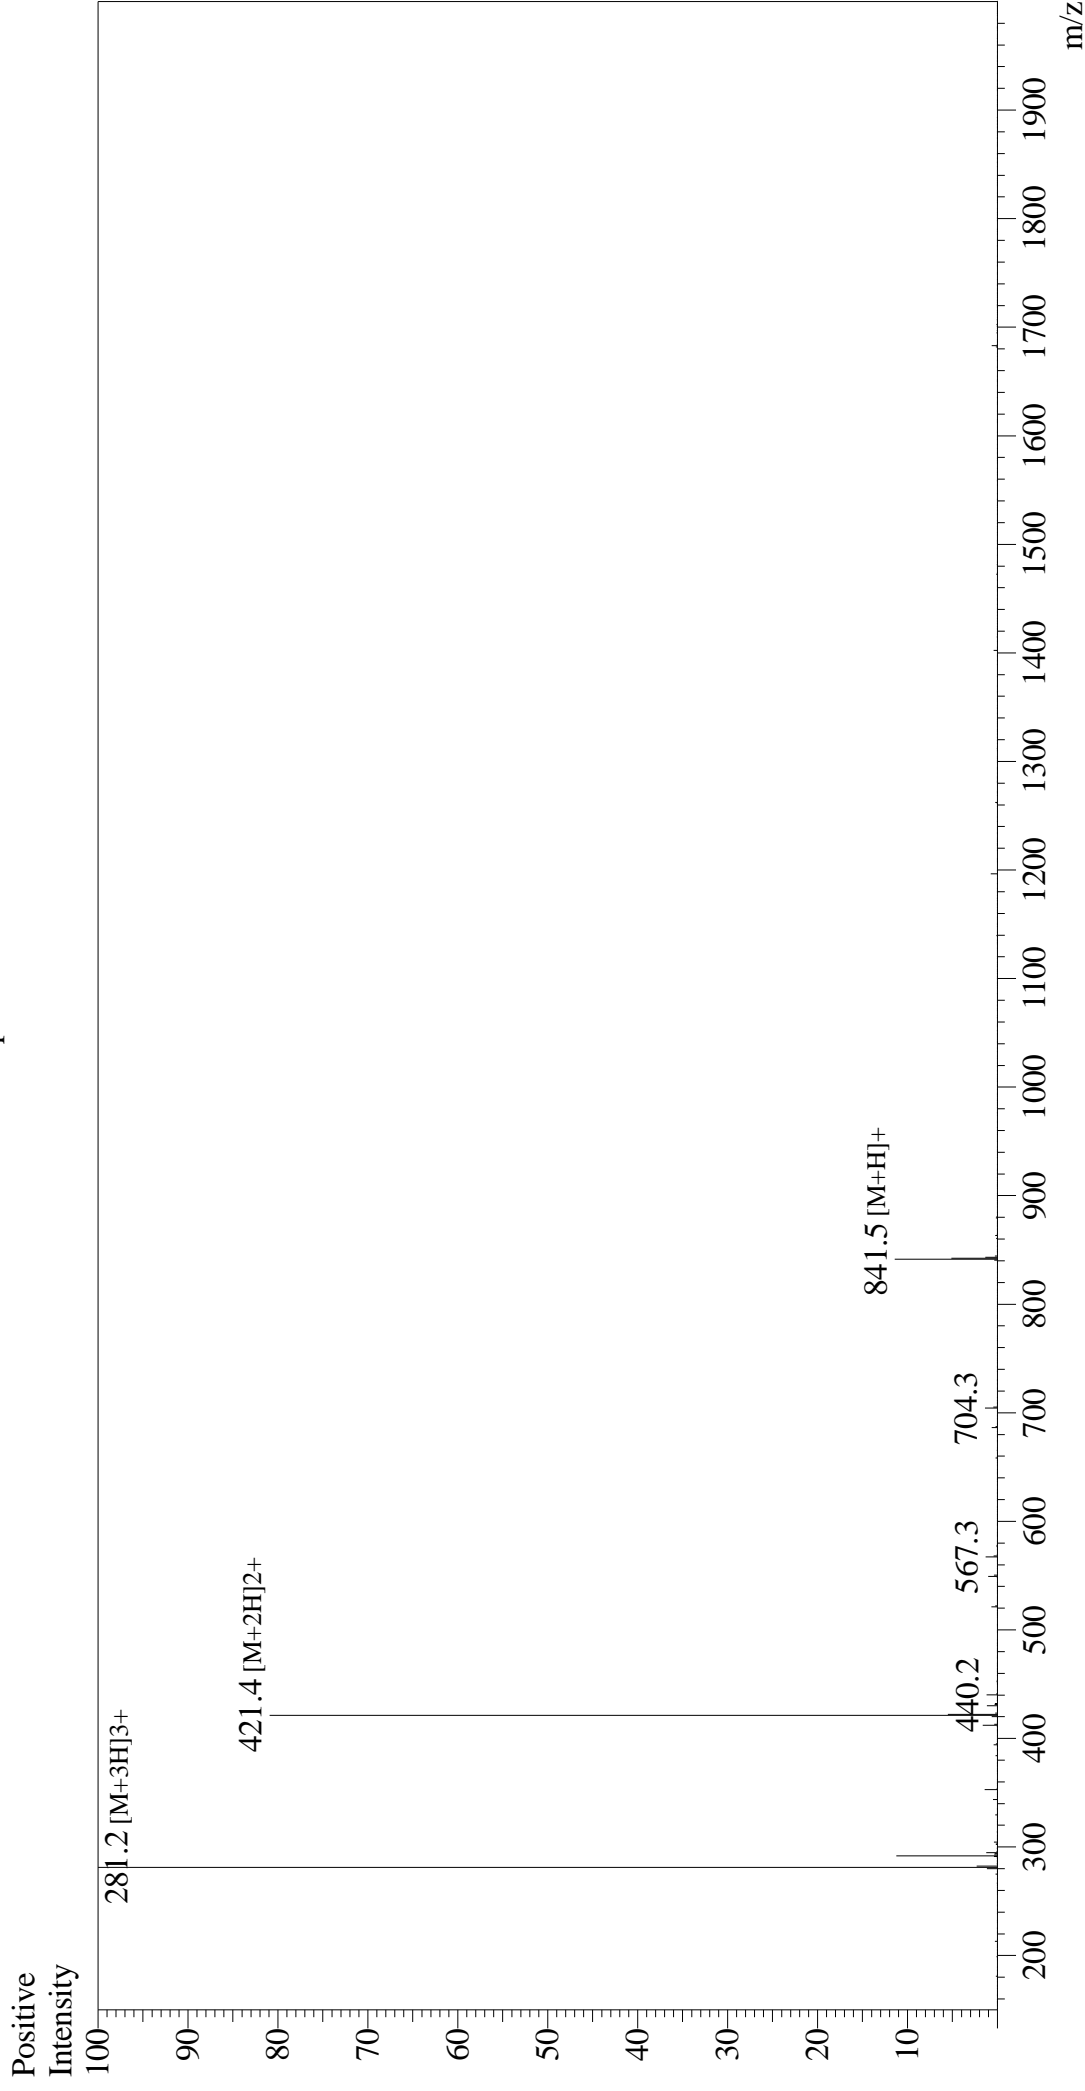

Sample Information

Month-Day Processed : 09/15/24
Time Processed : 21:42:26
Injection Volume : 0.4
Sample Name : Hexa-His

Cat No. : RP11737
Lot No. : E8758024I
Theoretical MW : 840.85
Observed MW : 840.6

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : ZJ21010035
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H₂O/50% MeOH