


Mass Spectrum

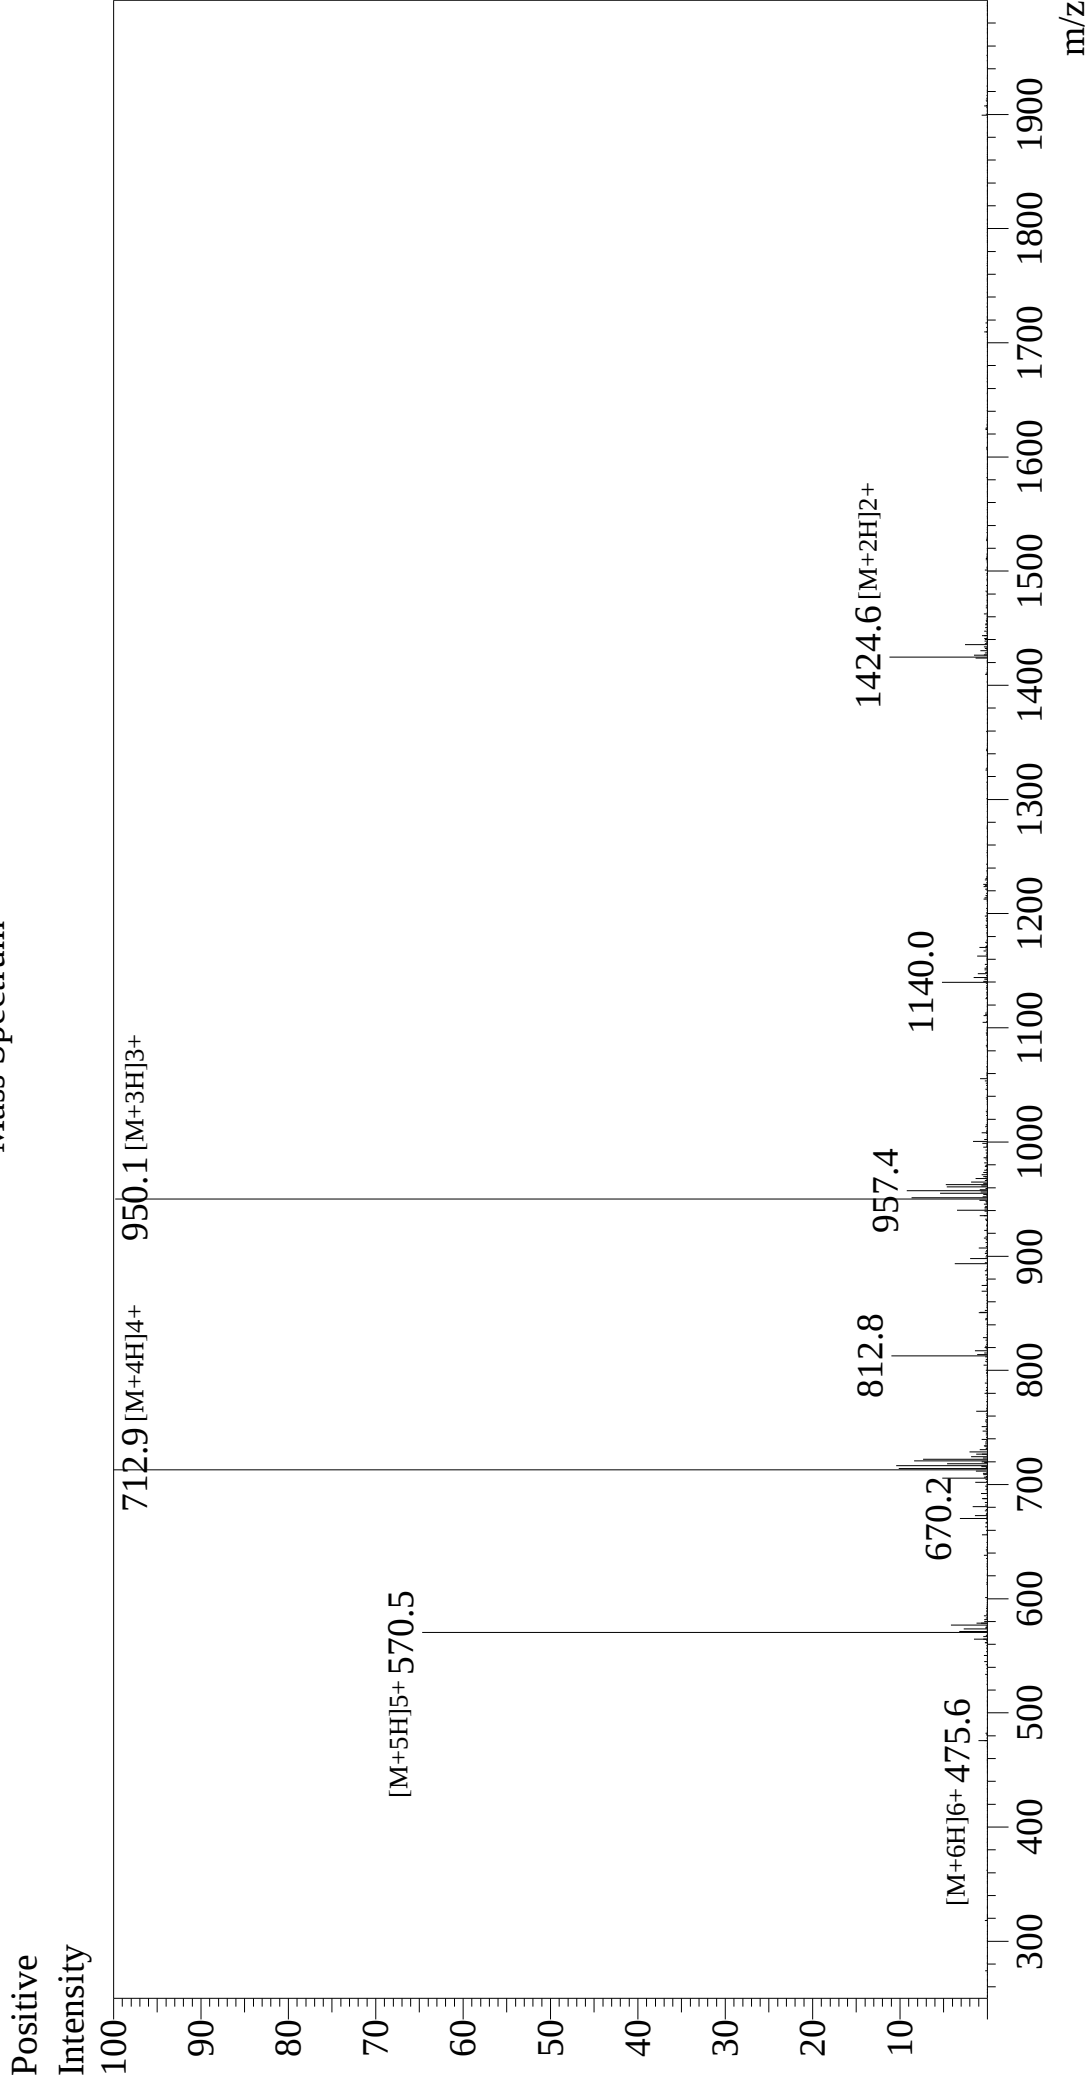

Sample Information		Interface	:ESI	Equipment	:ZJ22010150
Month-Day Processed :	04/23/25	Nebulizing Gas Flow	:1.5L/min	Interface Bias	: +4.5 kV
Time Processed :	1:05:39 PM	CDL Temp	:250	Drying Gas Flow	:5 L/min
Injection Volume :	0.2	Block Temp	:200	T.Flow	:0.2 ml/min
Sample Name :	Melittin,honey bee			B.conc	:50%H2O/50%MeOH
Cat No. :	RP20415				
Lot No. :	E8901625D				
Theoretical MW:	2847.50				
Observed MW :	2847.6				