


Mass Spectrum

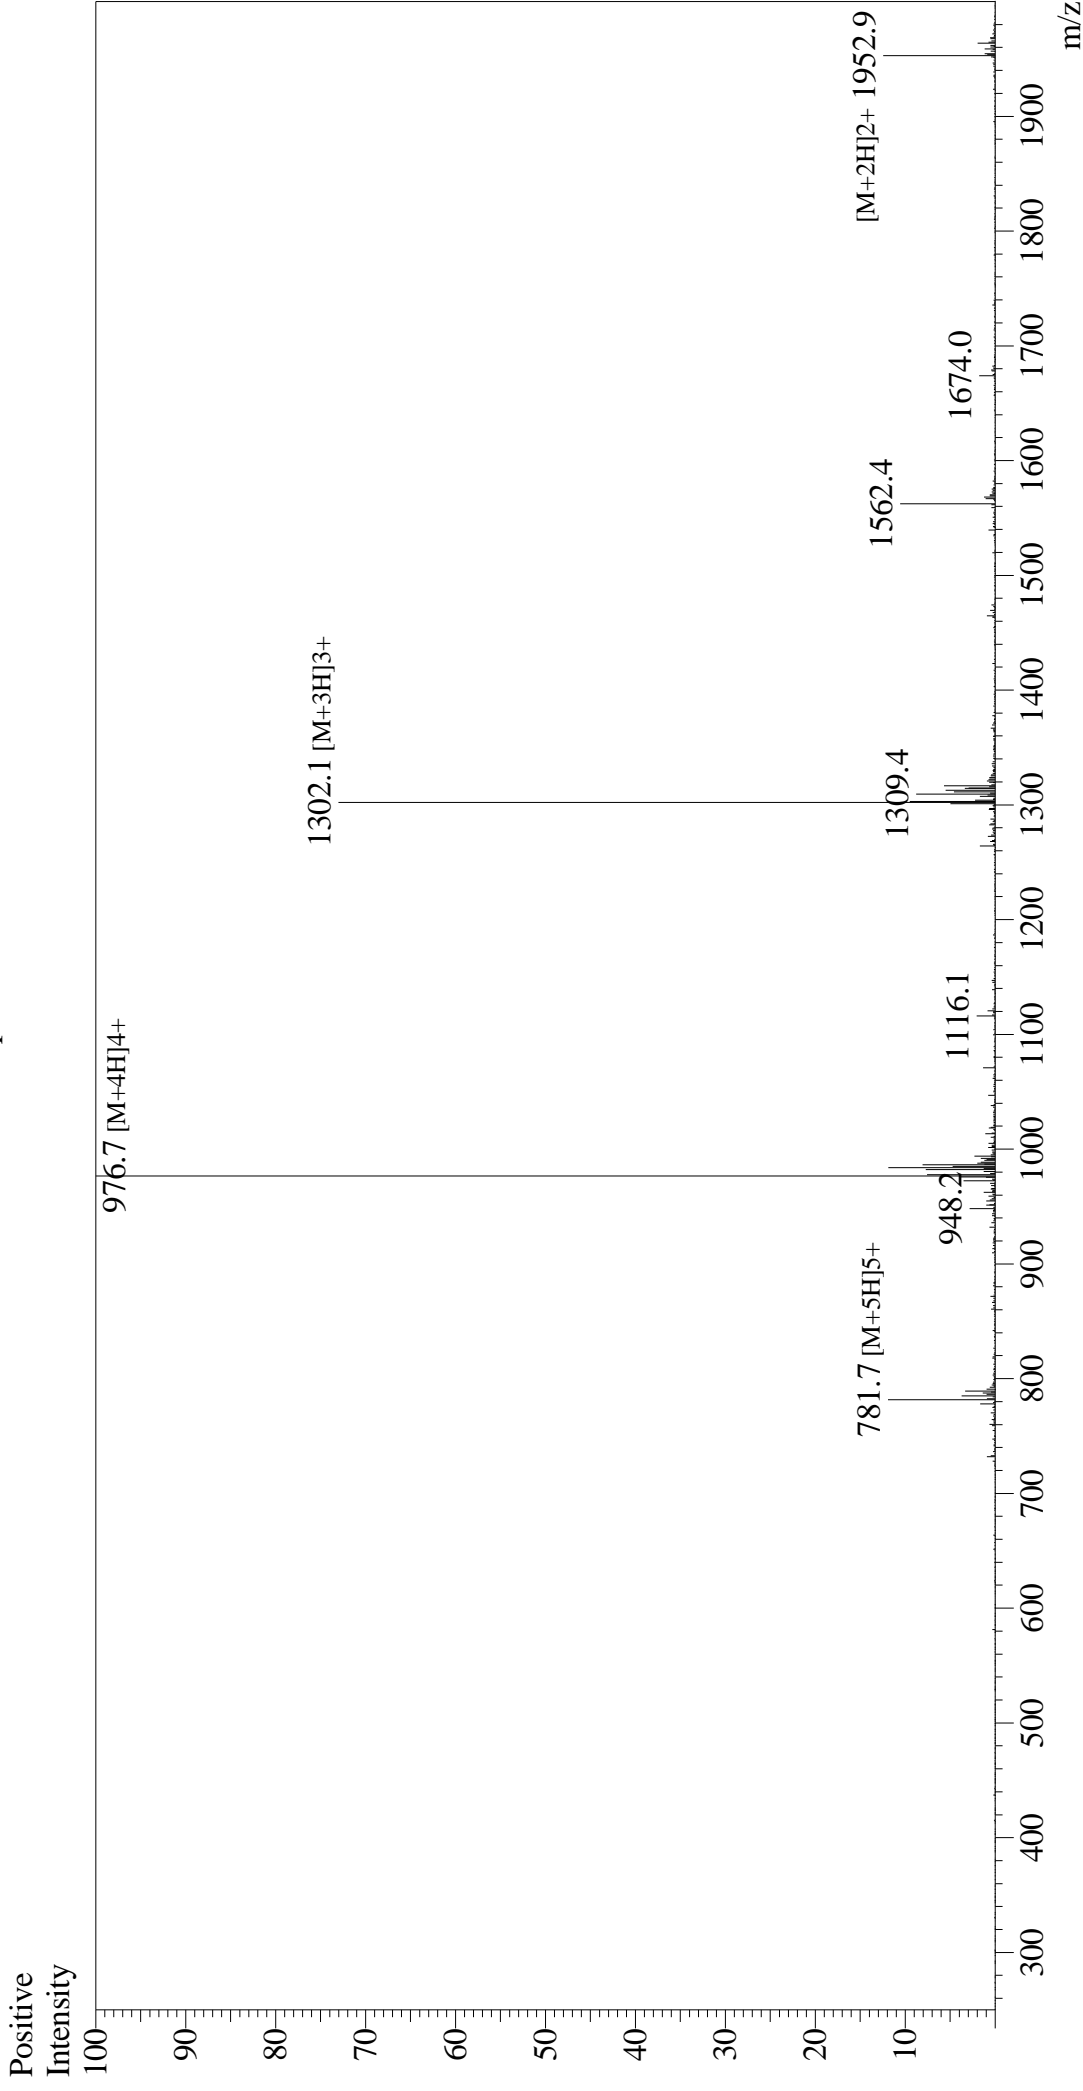

Sample Information

Month-Day Processed : 07/15/25
 Time Processed : 14:00:01
 Injection Volume : 0.2
 Sample Name : Amylin, human, amide
 Cat No. : RP11278
 Lot No. : E8908625G
 Theoretical MW : 3903.28
 Observed MW : 3902.8

Interface

Interface : ESI
 Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200

Equipment

Equipment : ZJ21010035
 Interface Bias : +4.5 kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2 ml/min
 B.conc : 50% H₂O/50% MeOH