

Sample Name :Substance P  
 Cat No. : RP10178  
 Lot No. : E8973523C  
 Time Processed :7:48:43  
 Month-Day-Year Processed :03/28/2023

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010140

### <Chromatogram>

mV

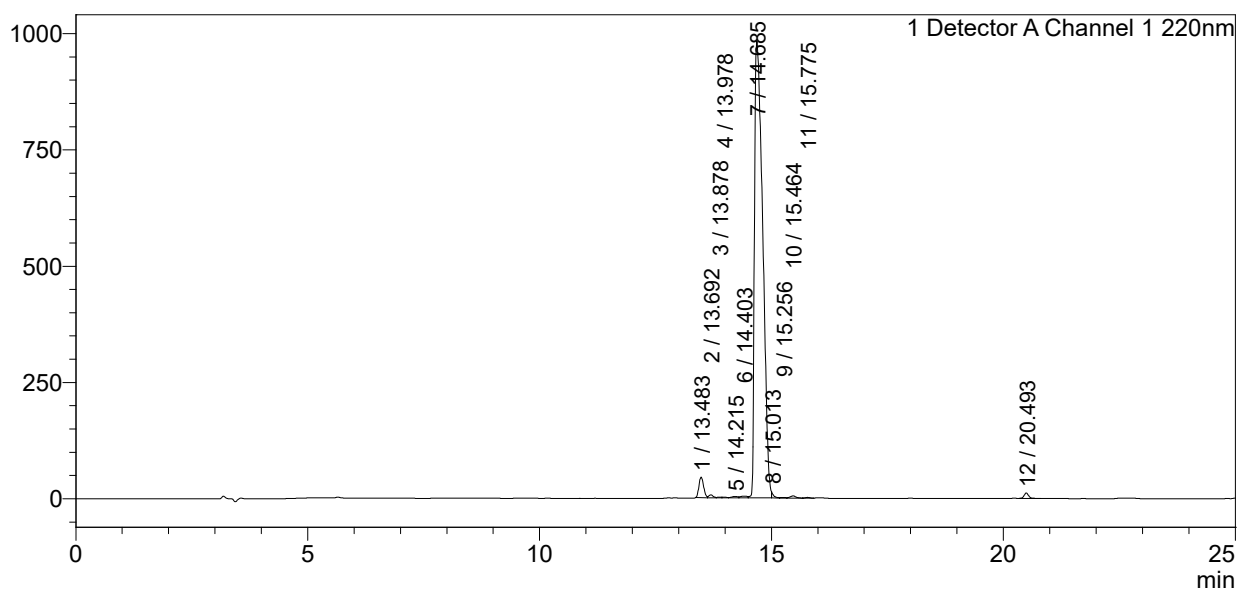

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.483	311231	44282	2.455
2	13.692	38027	6149	0.300
3	13.878	7747	1167	0.061
4	13.978	8465	1191	0.067
5	14.215	27959	2996	0.220
6	14.403	38276	3782	0.302
7	14.685	12073066	983162	95.214
8	15.013	36356	11520	0.287
9	15.256	9163	1230	0.072
10	15.464	40588	4689	0.320
11	15.775	10047	1683	0.079
12	20.493	79033	11750	0.623
Total		12679959	1073600	100.000