


Mass Spectrum

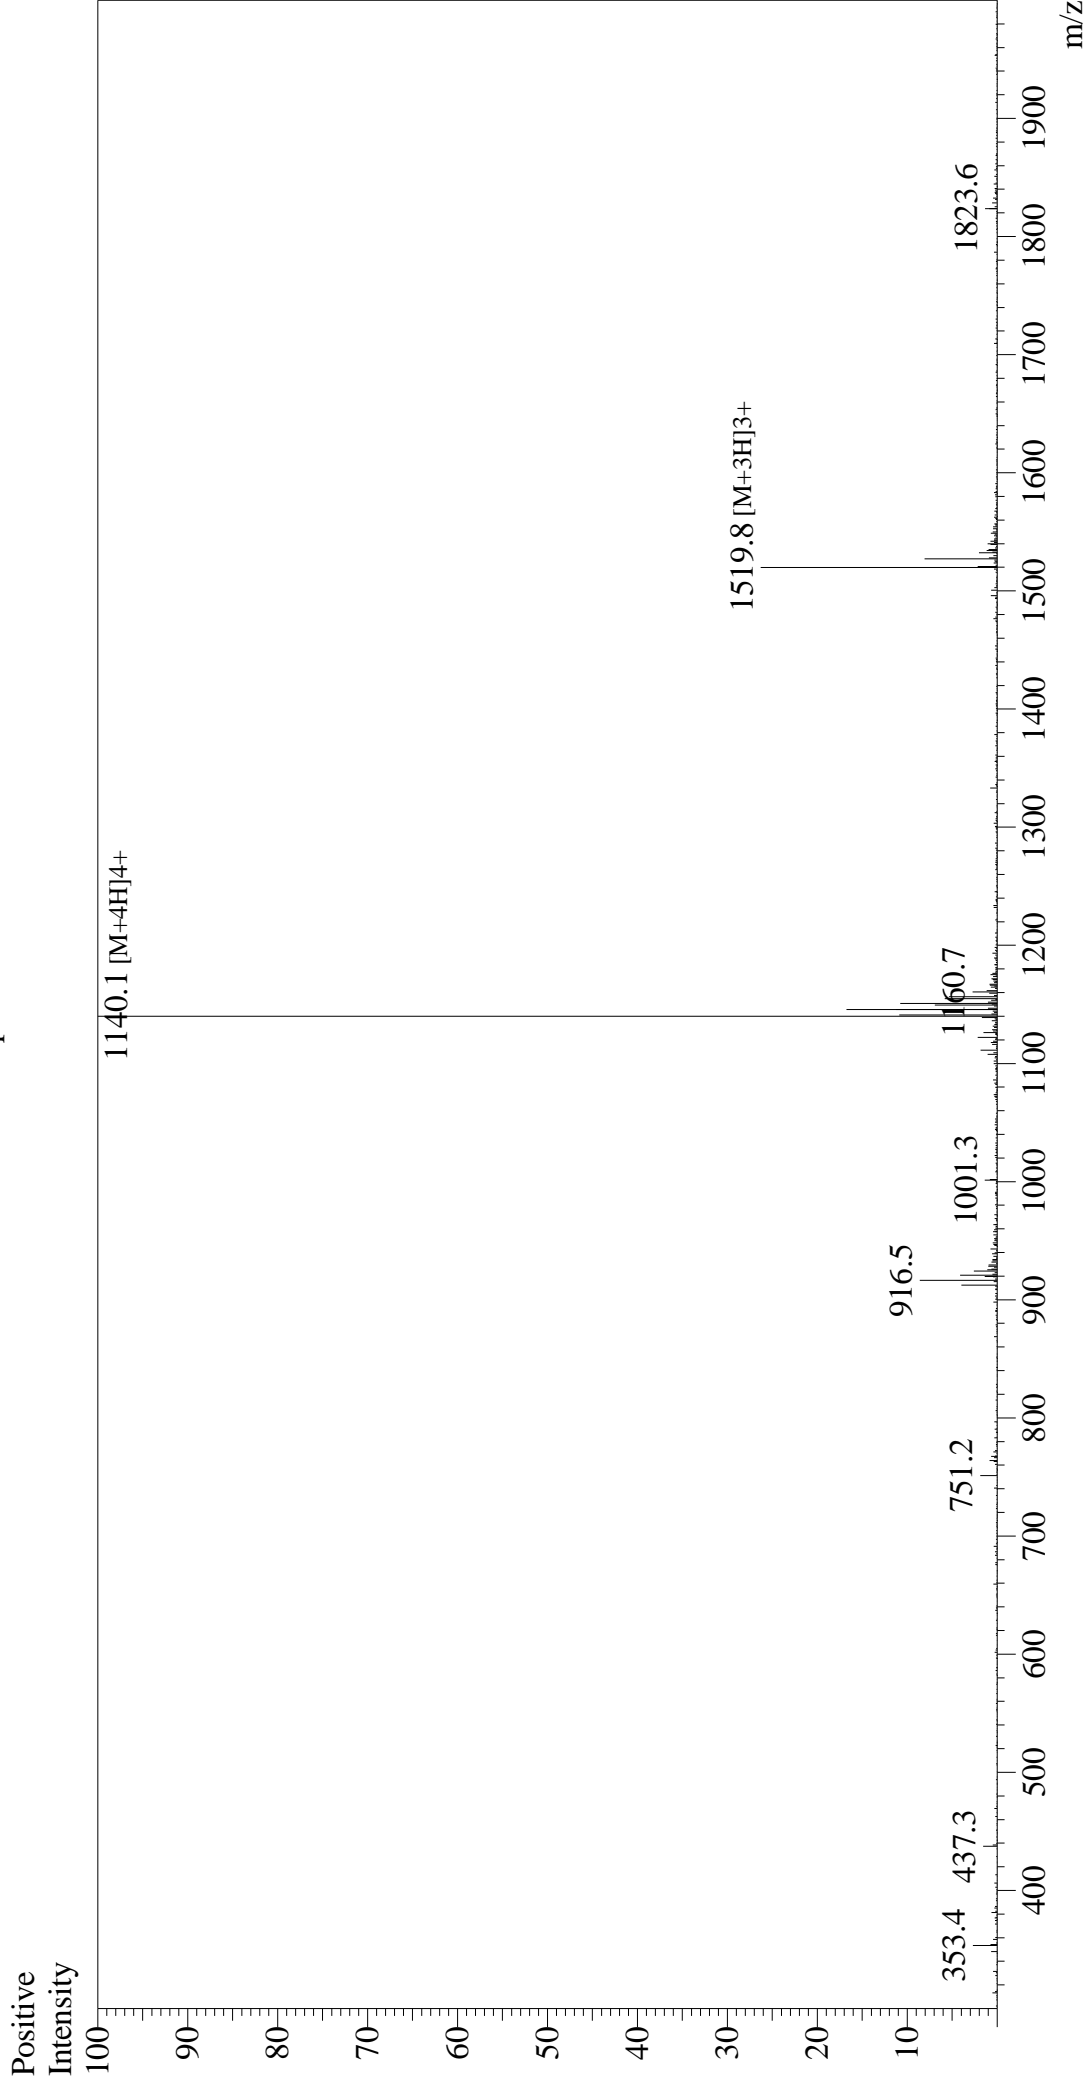

Sample Information

Month-Day Processed :	02/21/24	Equipment	:ZJ22010150
Time Processed :	10:16:55 AM	Interface Bias	:+4.5 kV
Injection Volume :	0.2	Drying Gas Flow	:5 L/min
Sample Name :	Biotin-β-Amyloid (1-40)	T.Flow	:0.2 ml/min
Cat No. :	RP30249	B.conc	:50%H2O/50%MeOH
Lot No. :	E8987424G		
Theoretical MW:	4556.12		
Observed MW :	4556.4		