


Mass Spectrum

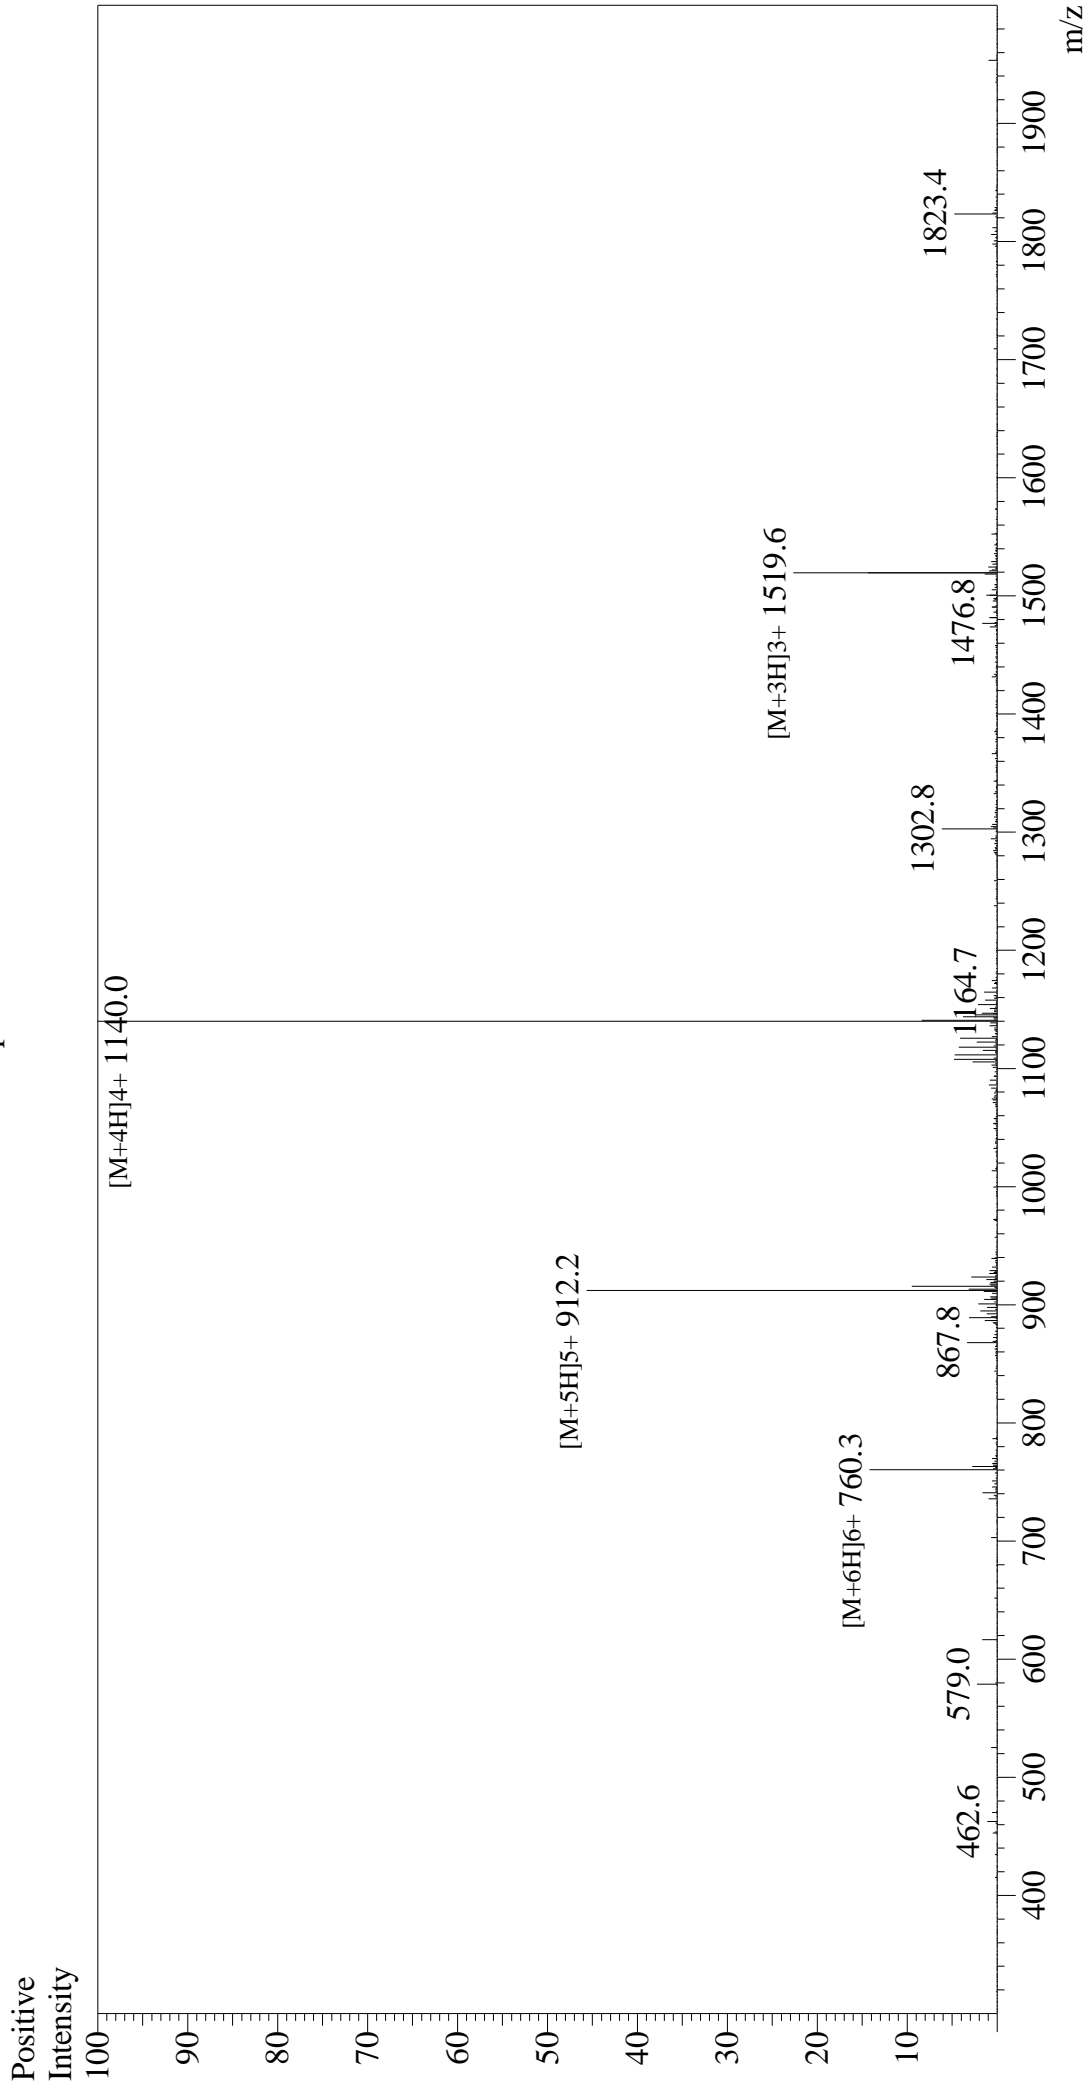

Sample Information

Month-Day Processed : 04/17/26
Time Processed : 22:22:05
Injection Volume : 0.8
Sample Name : Biotin- β -Amyloid (1-40)
Cat No. : RP30249
Lot No. : E9007026D

Interface

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment

Equipment : ZJ22010150
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H₂O/50% MeOH

Theoretical MW: 4556.12

Observed MW : 4556.0