


Mass Spectrum

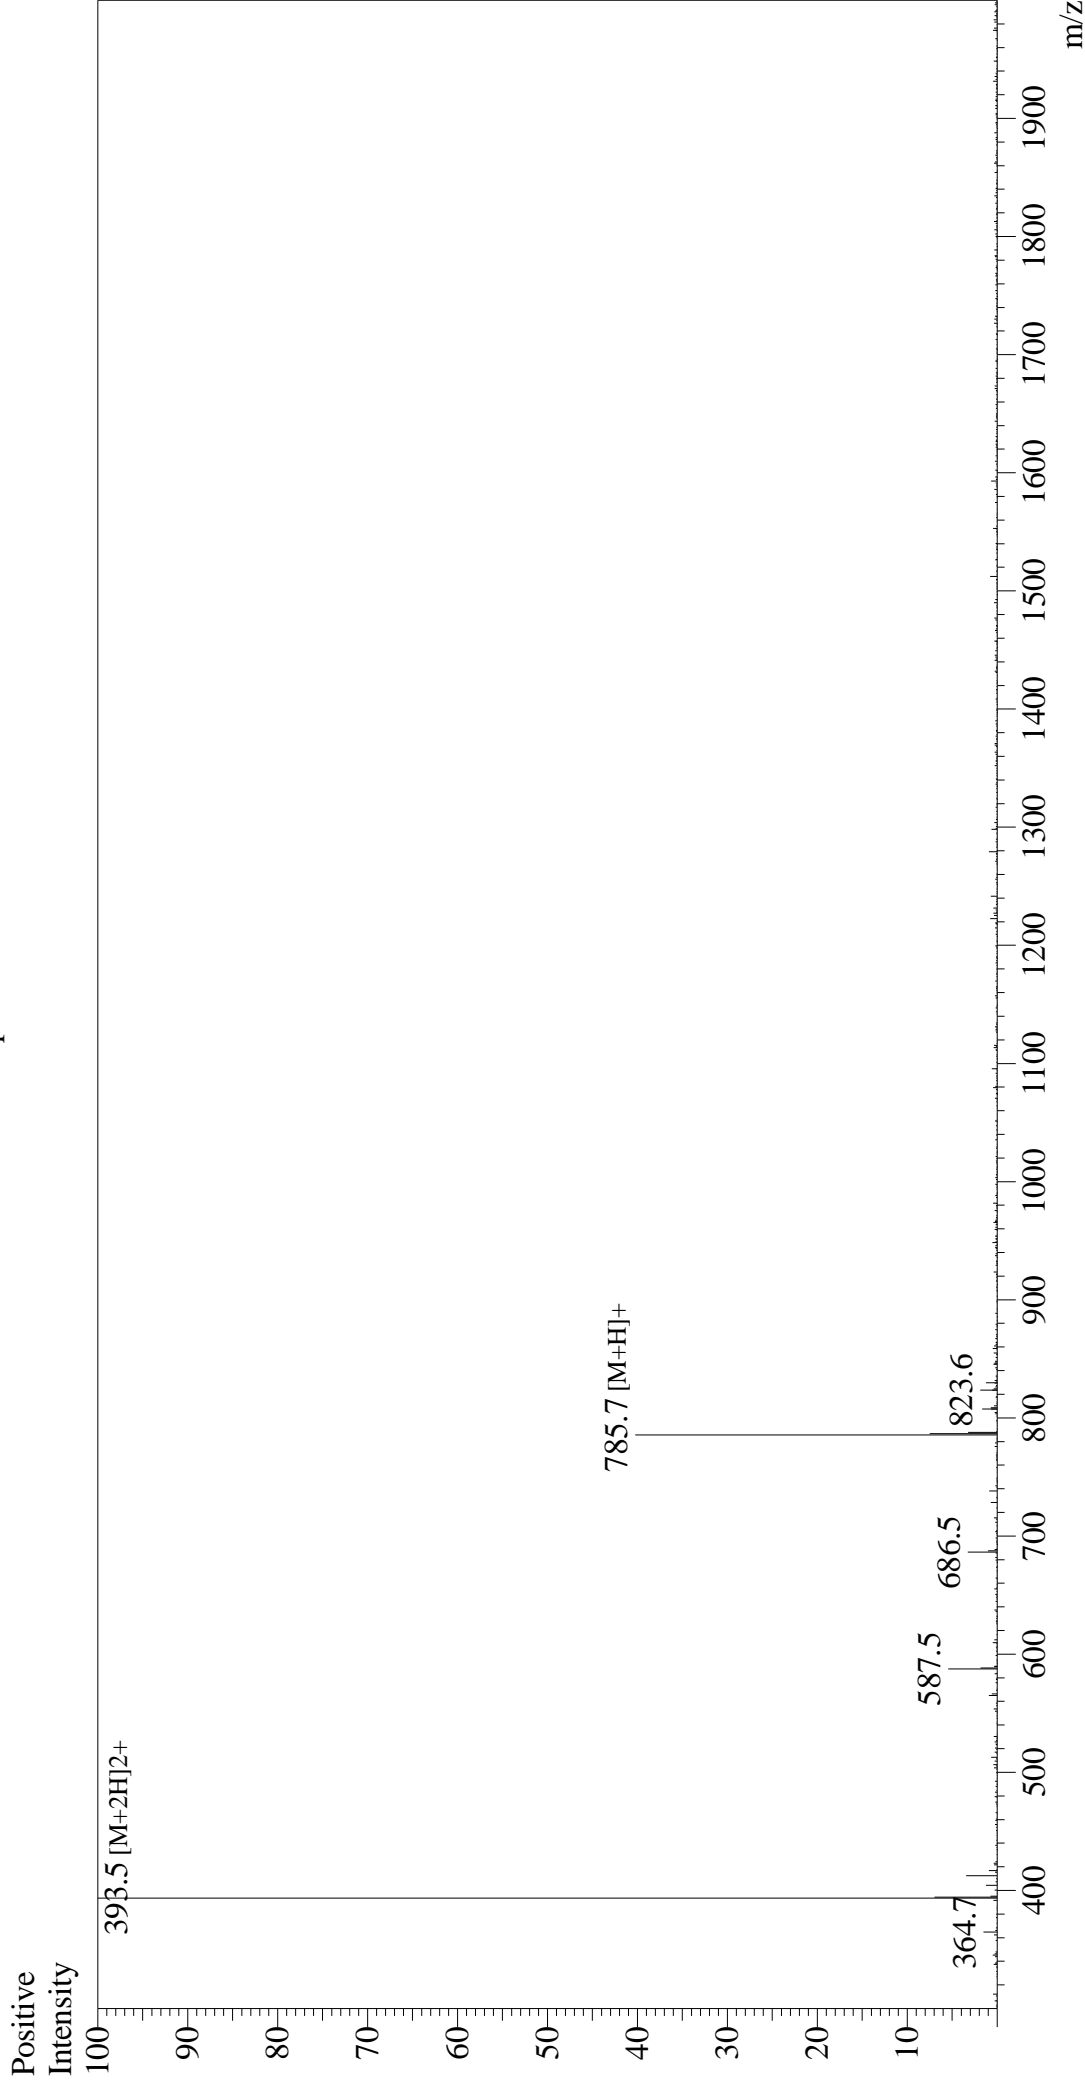

Sample Information

Month-Day Processed : 03/27/23

Time Processed : 17:41:58

Injection Volume : 0.1

Sample Name : KRAS G12V Peptide (VVGAVGVGK)

Cat No. : RP30228

Lot No. : E9071823C

Theoretical MW: 784.95

Observed MW : 785.0

Interface

Nebulizing Gas Flow : 1.5L/min

CDL Temp : 250

Block Temp : 200

Equipment

Interface Bias

Drying Gas Flow

T.Flow

B.conc

:ZJ22010150

: +4.5 kV

: 5 L/min

: 0.2 ml/min

: 50% H₂O / 50% MeOH