


Mass Spectrum

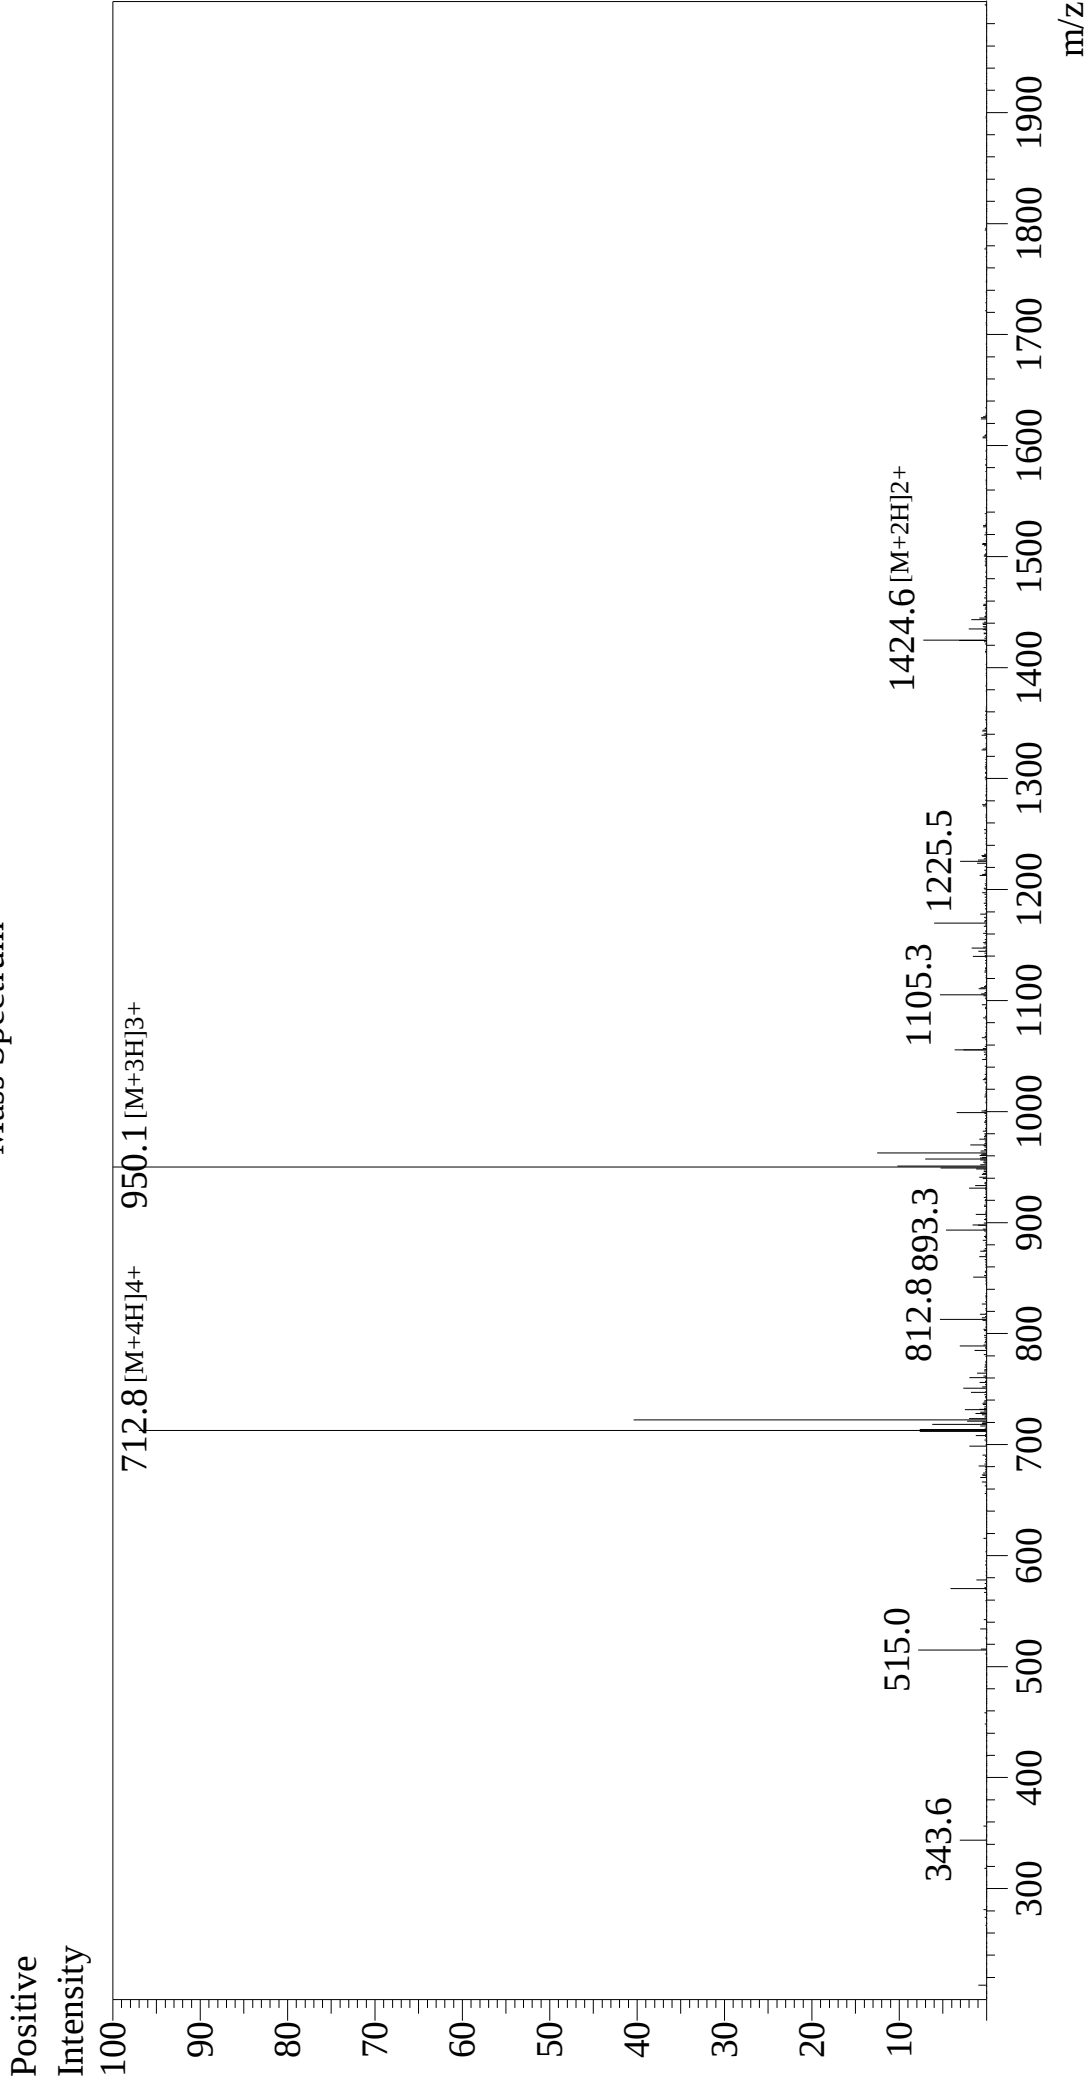

Sample Information

Month-Day Processed : 09/28/24
 Time Processed : 2:05:33 PM
 Injection Volume : 0.5
 Sample Name : Melittin,honey bee
 Cat No. : RP20415
 Lot No. : E9207424I
 Theoretical MW : 2847.50
 Observed MW : 2847.3

Interface :ESI

Nebulizing Gas Flow :1.5L/min
 CDL Temp :250
 Block Temp :200

Equipment

Interface Bias :+4.5 kV
 Drying Gas Flow :5 L/min
 T.Flow :0.2 ml/min
 B.conc :50%H₂O/50%MeOH

Equipment : ZJ21010035