


Mass Spectrum

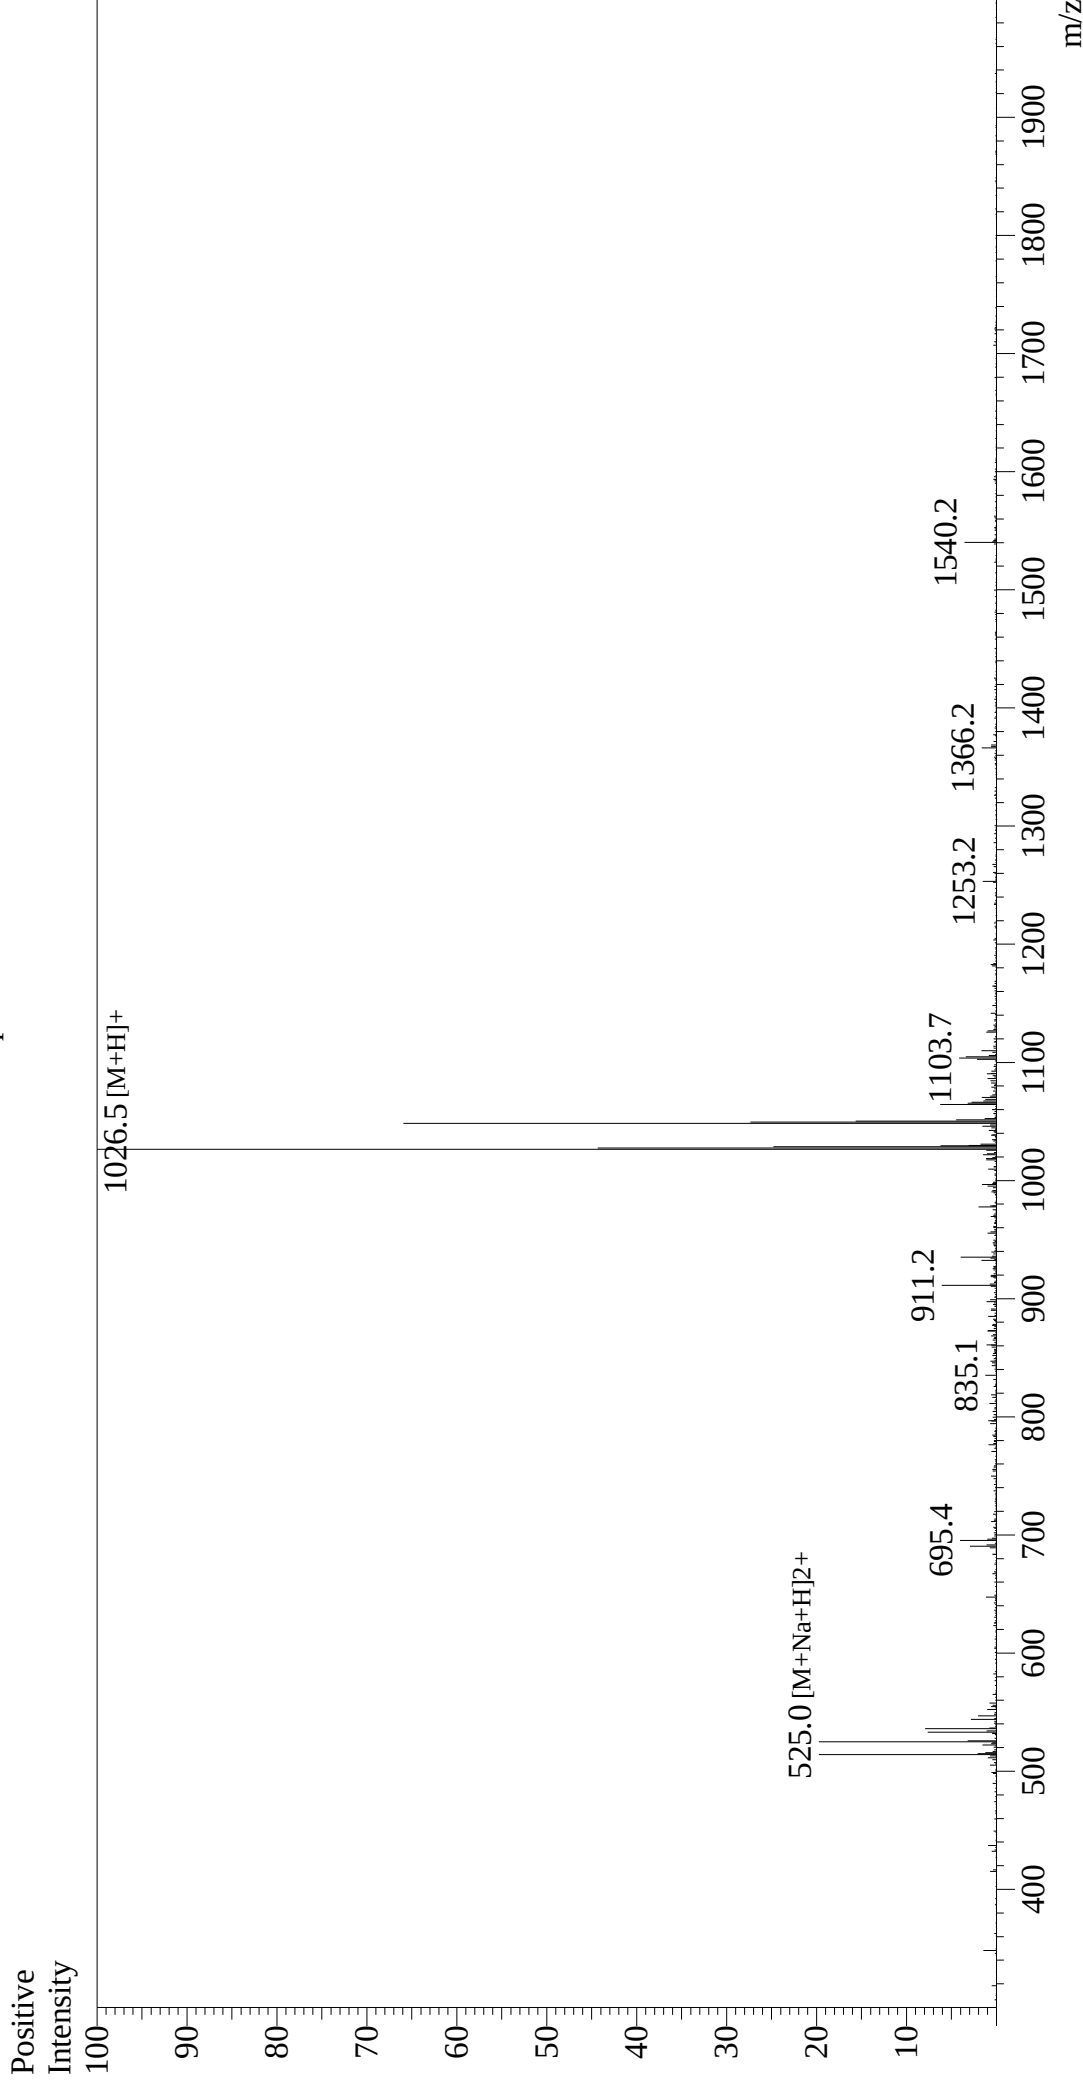

Sample Information

Month-Day Processed :	03/20/24	Equipment	:ZJ22010150
Time Processed :	10:47:54 AM	Interface Bias	: +4.5 kV
Injection Volume :	0.3	Drying Gas Flow	:5 L/min
Sample Name :	Influenza A NP(366-374) Strain A/PR/8/35	T.Flow	:0.2 ml/min
Cat No. :	RP20267	B.conc	:50%H2O/50%MeOH
Lot No. :	E9400724C		
Theoretical MW: 1026.12			
Observed MW : 1025.5			