

Sample Name :Substance P  
Cat No. : RP10178  
Lot No. : E9471825C  
Time Processed :5:27:25  
Month-Day-Year Processed :04/01/2025

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
Total Flow:1 ml/min  
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ19010142

### <Chromatogram>

mV

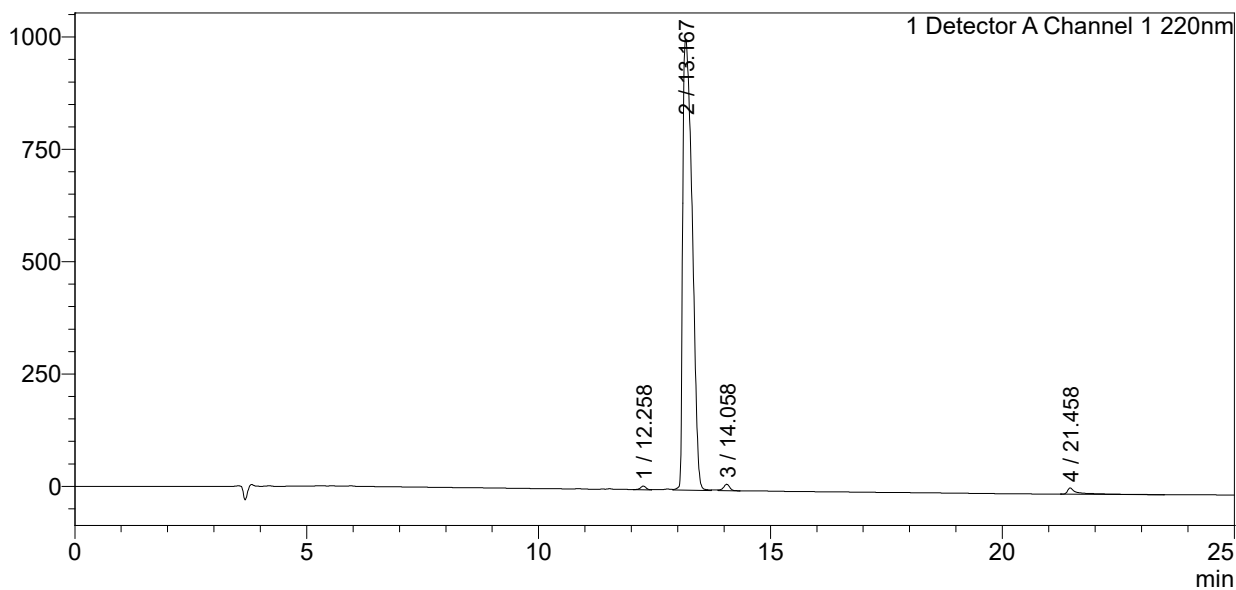

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.258	64624	8062	0.442
2	13.167	14165596	1004697	96.984
3	14.058	131888	14218	0.903
4	21.458	243968	14010	1.670
Total		14606076	1040986	100.000