


Mass Spectrum

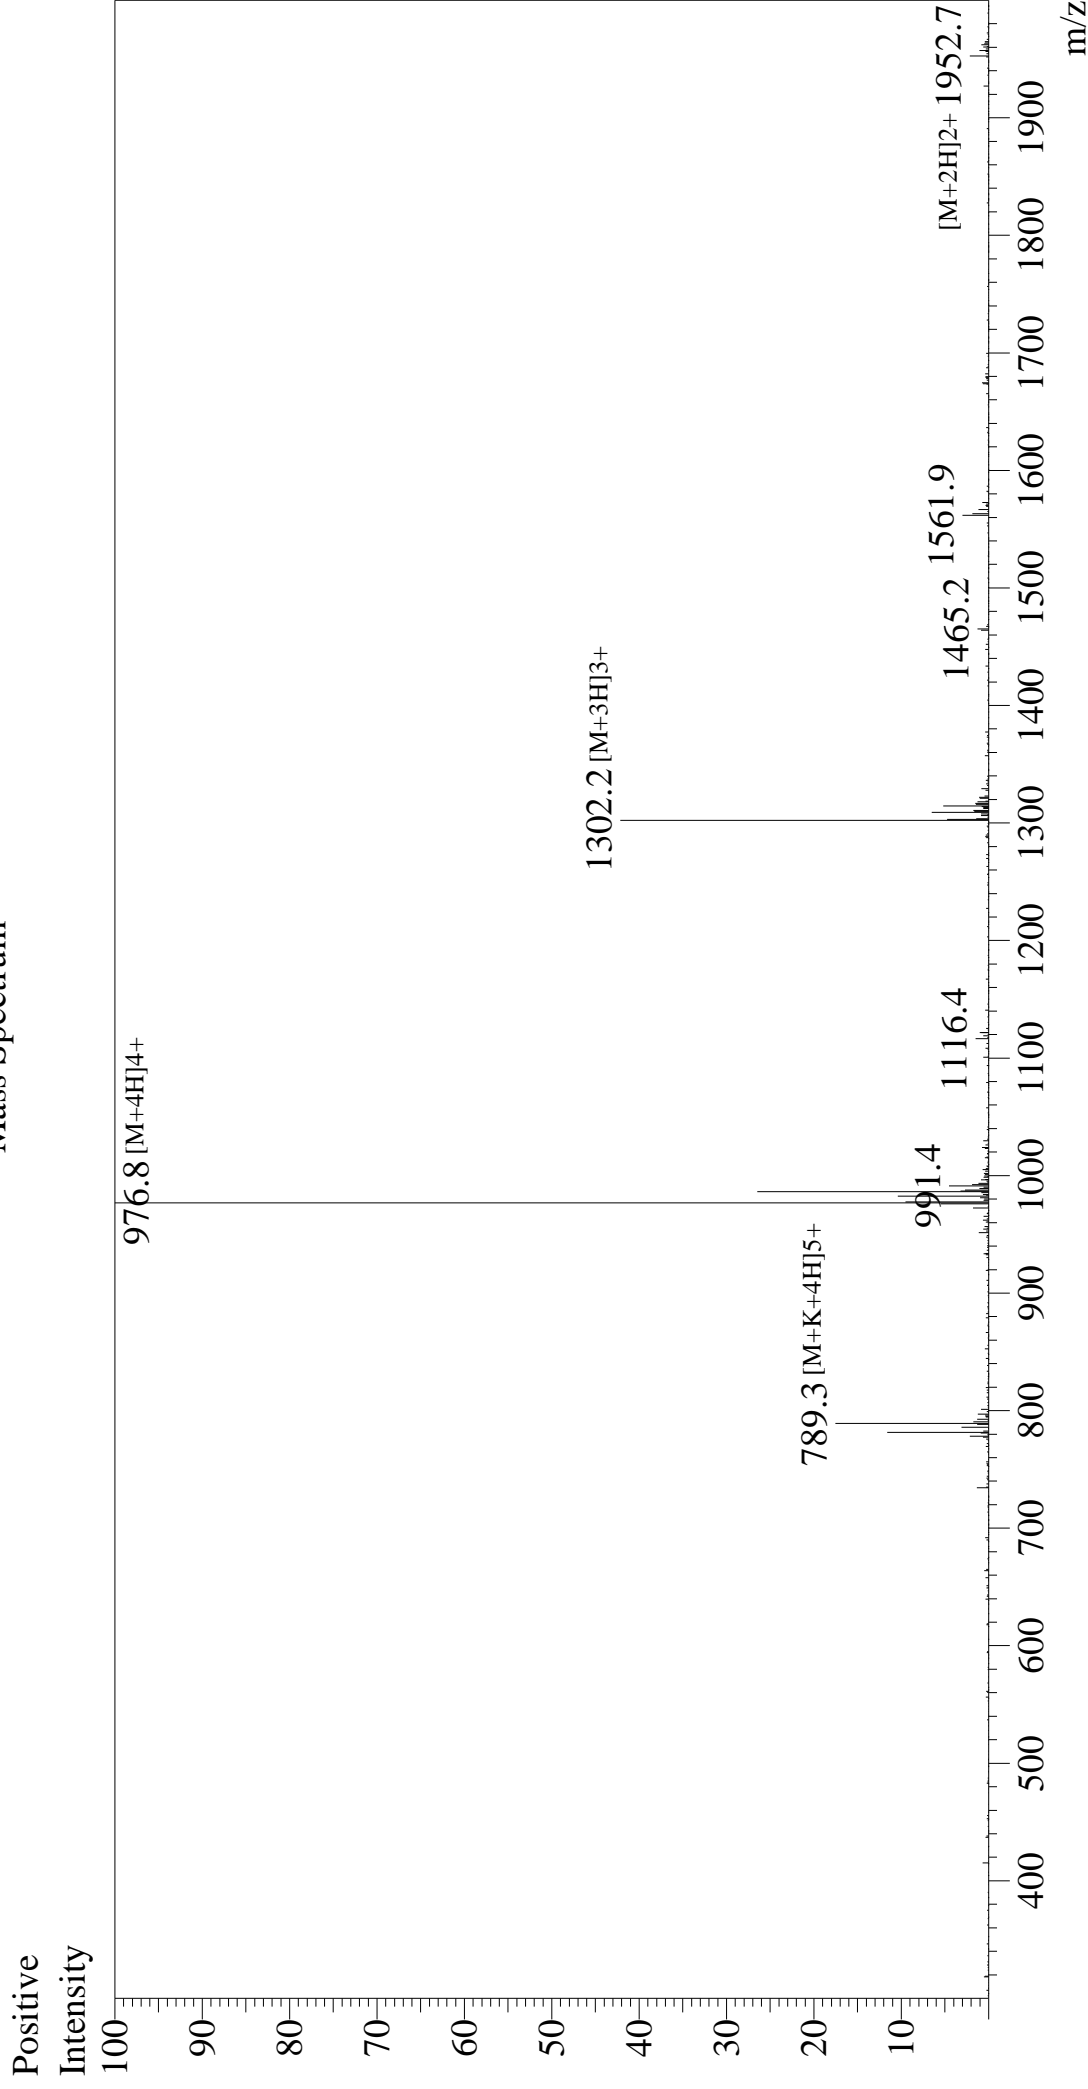

Sample Information

Month-Day Processed : 06/25/24
Time Processed : 18:43:30
Injection Volume : 0.2
Sample Name : Amylin, human, amide
Cat No. : RP11278
Lot No. : E9498824F
Theoretical MW : 3903.28
Observed MW : 3903.2

Interface

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment

Equipment : ZI21010035
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH