


Mass Spectrum

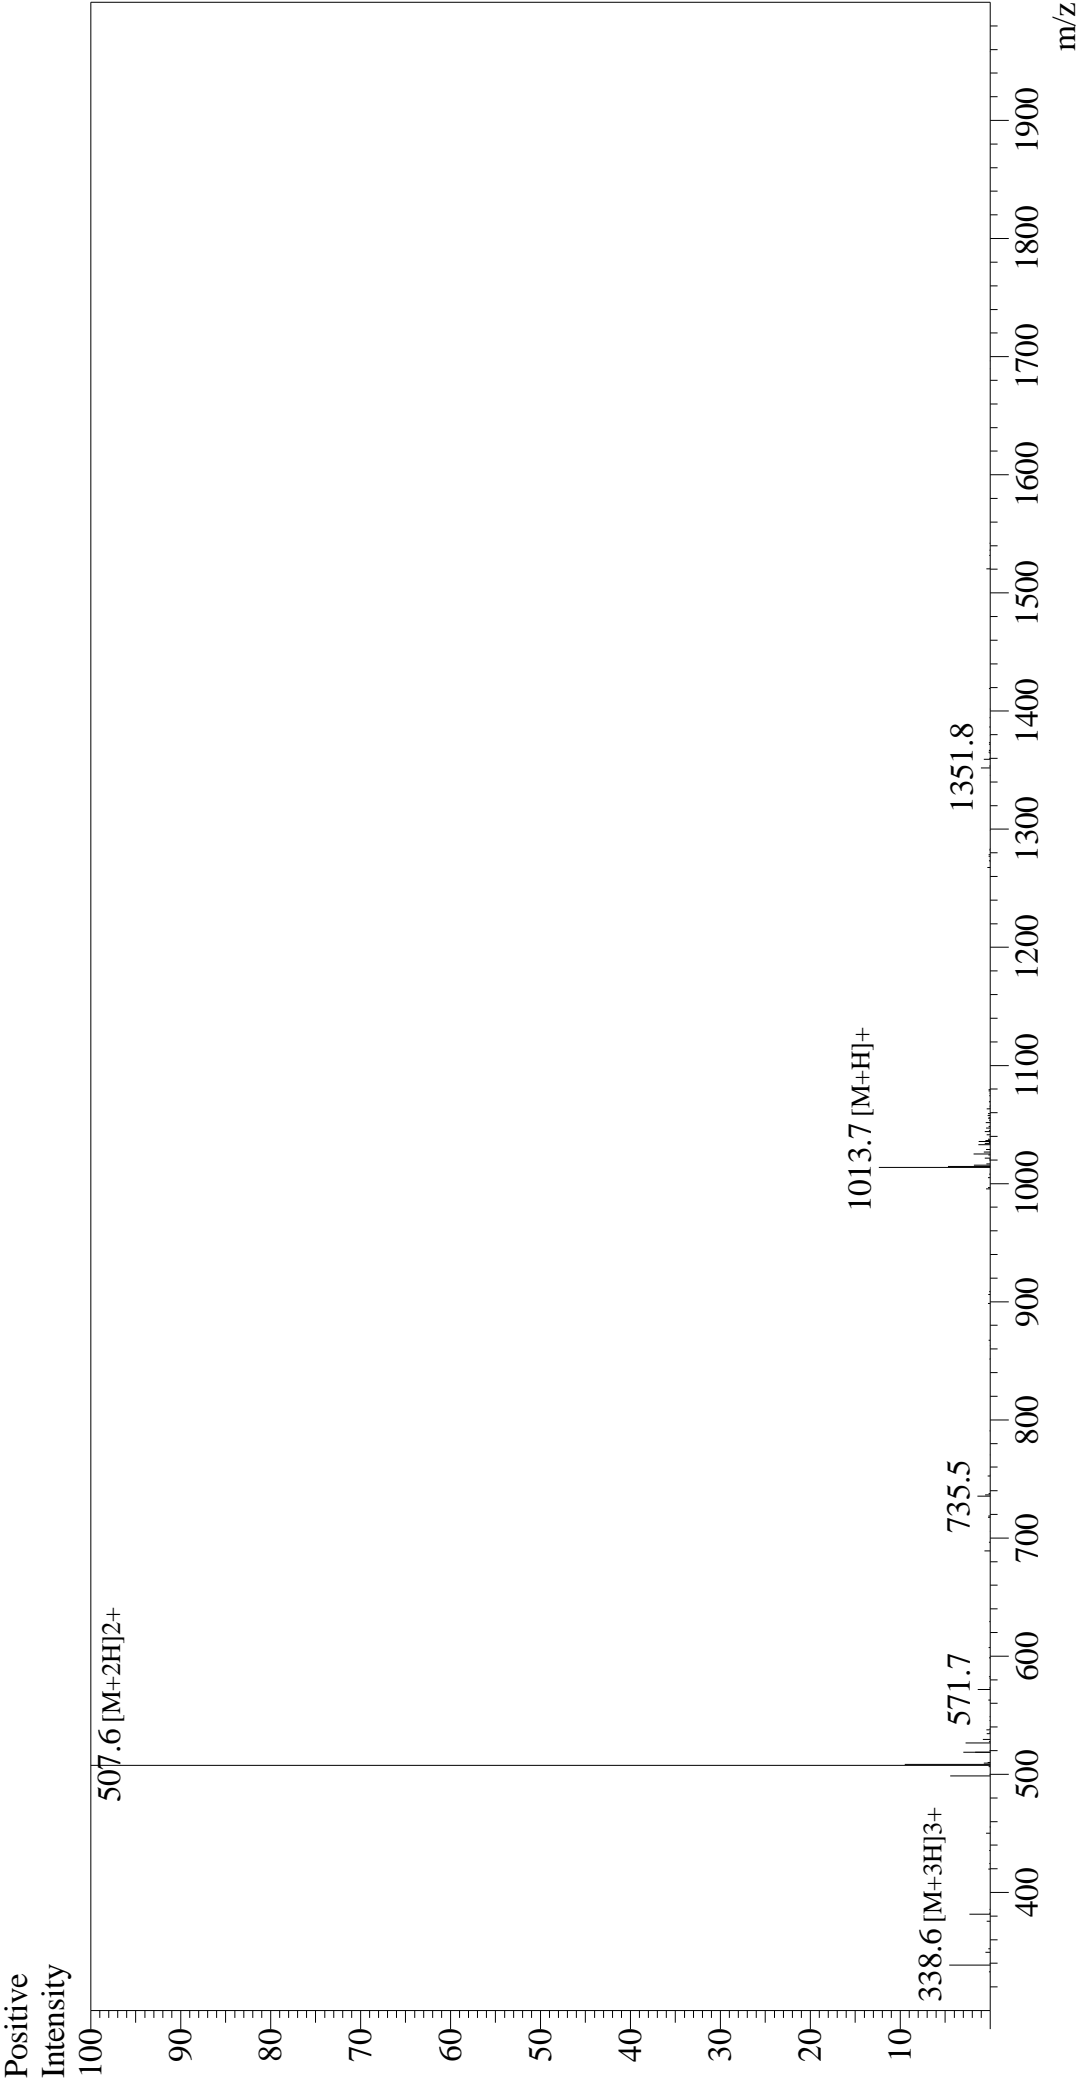

Sample Information

Month-Day Processed :	08/17/22	Equipment	:ZJ22010150
Time Processed :	19:38:58	Interface Bias	:+4.5 kV
Injection Volume :	0.1	Drying Gas Flow	:5 L/min
Sample Name :	DYKDDDDK Peptide	T.Flow	:0.2 ml/min
Cat No. :	RP10586	B.conc	:50%H2O/50%MeOH
Lot No. :	E9546022H		
Theoretical MW :	1012.97		
Observed MW :	1013.2		