

Sample Name :Substance P
Cat No. : RP10178
Lot No. : E9639722F
Time Processed :7:48:45 AM
Month-Day-Year Processed :06/28/2022

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm
Equipment: ZJ19010141

<Chromatogram>

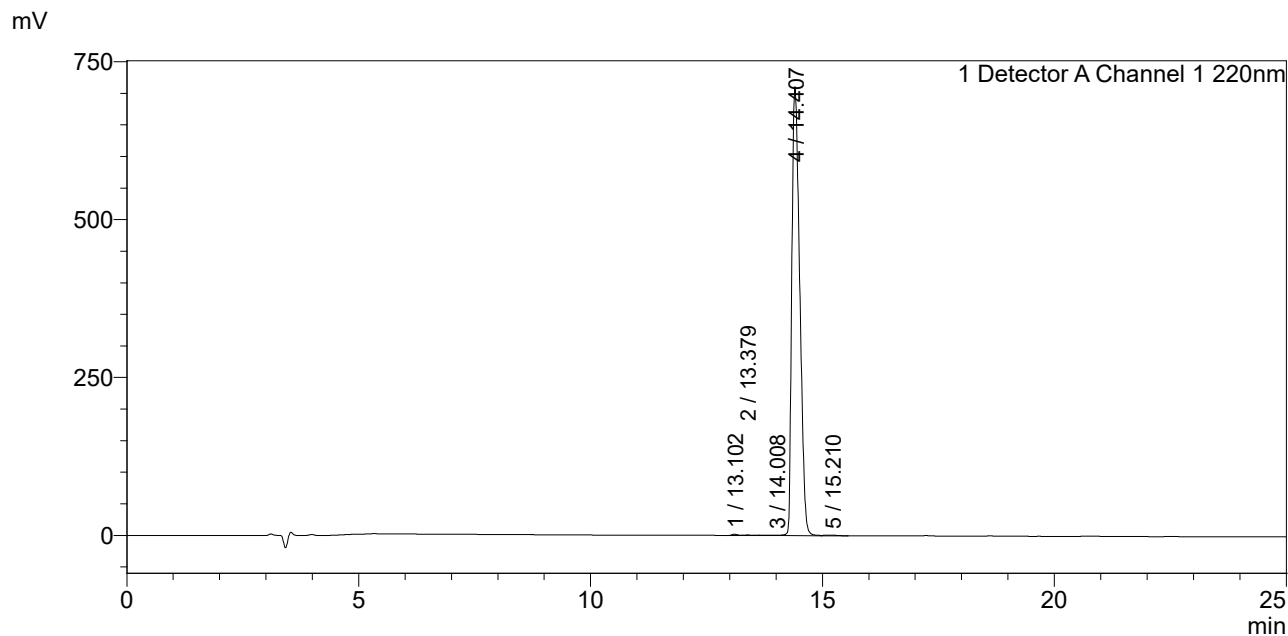

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.102	19353	2085	0.227
2	13.379	14438	977	0.170
3	14.008	20418	862	0.240
4	14.407	8436274	711036	99.149
5	15.210	18242	1049	0.214
Total		8508726	716008	100.000