

Sample Name :C-Type Natriuretic Peptide (CNP) (1-22), human

Cat No. : RP11110

Lot No. : E9705525D

Time Processed :21:43:57

Month-Day-Year Processed :04/26/2025

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm

Equipment: ZJ19010142

<Chromatogram>

mV

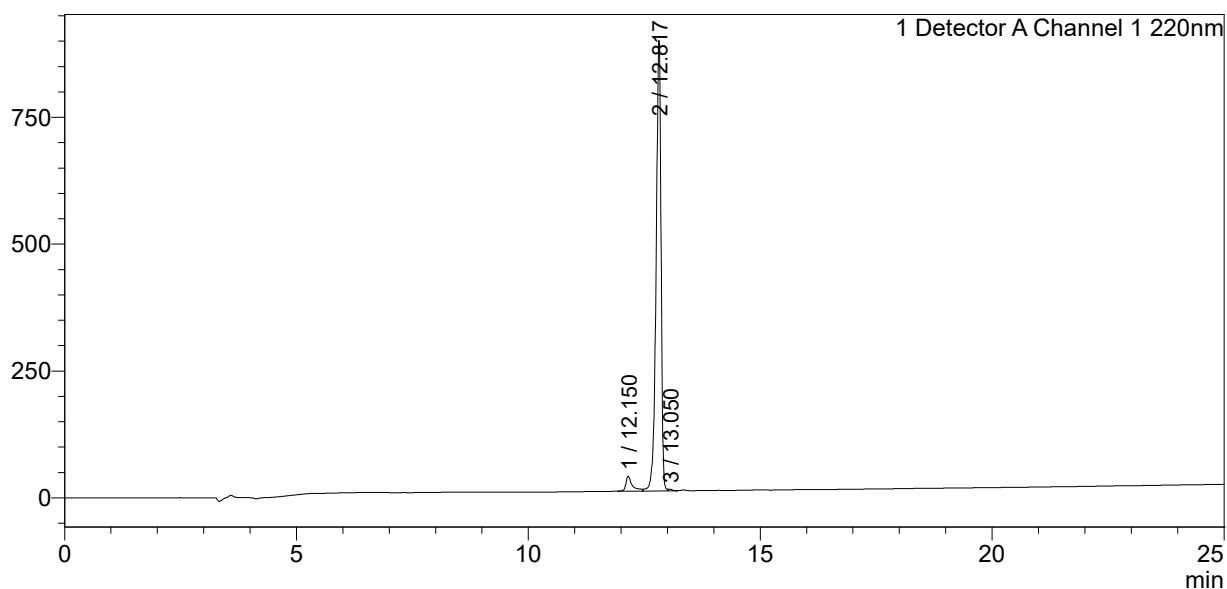

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.150	282732	29518	4.096
2	12.817	6599623	888091	95.615
3	13.050	19907	3070	0.288
Total		6902262	920679	100.000