

Sample Name :Biotin-β-Amyloid (1-40)  
 Cat No. :RP30249  
 Lot No. :E9708225H  
 Time Processed :13:18:41  
 Month-Day-Year Processed :08/29/2025

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :UniPSN 30-300 30um,4.6x250mm

<Chromatogram>

mV

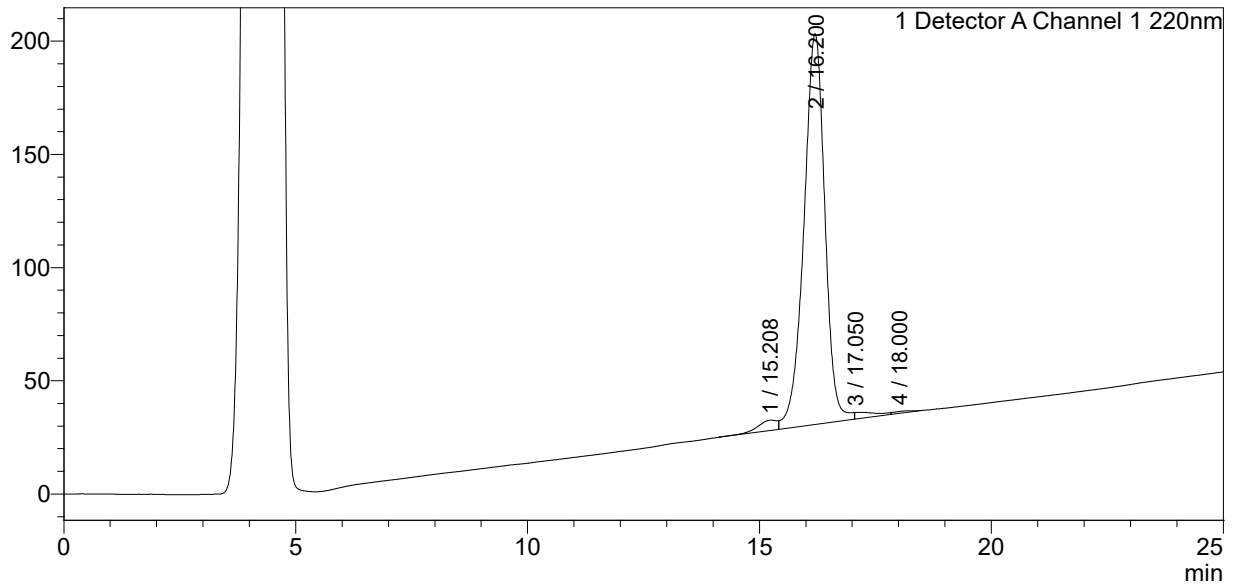

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.208	131844	4550	2.327
2	16.200	5427328	172664	95.790
3	17.050	84177	2996	1.486
4	18.000	22507	847	0.397
Total		5665857	181058	100.000