


Mass Spectrum

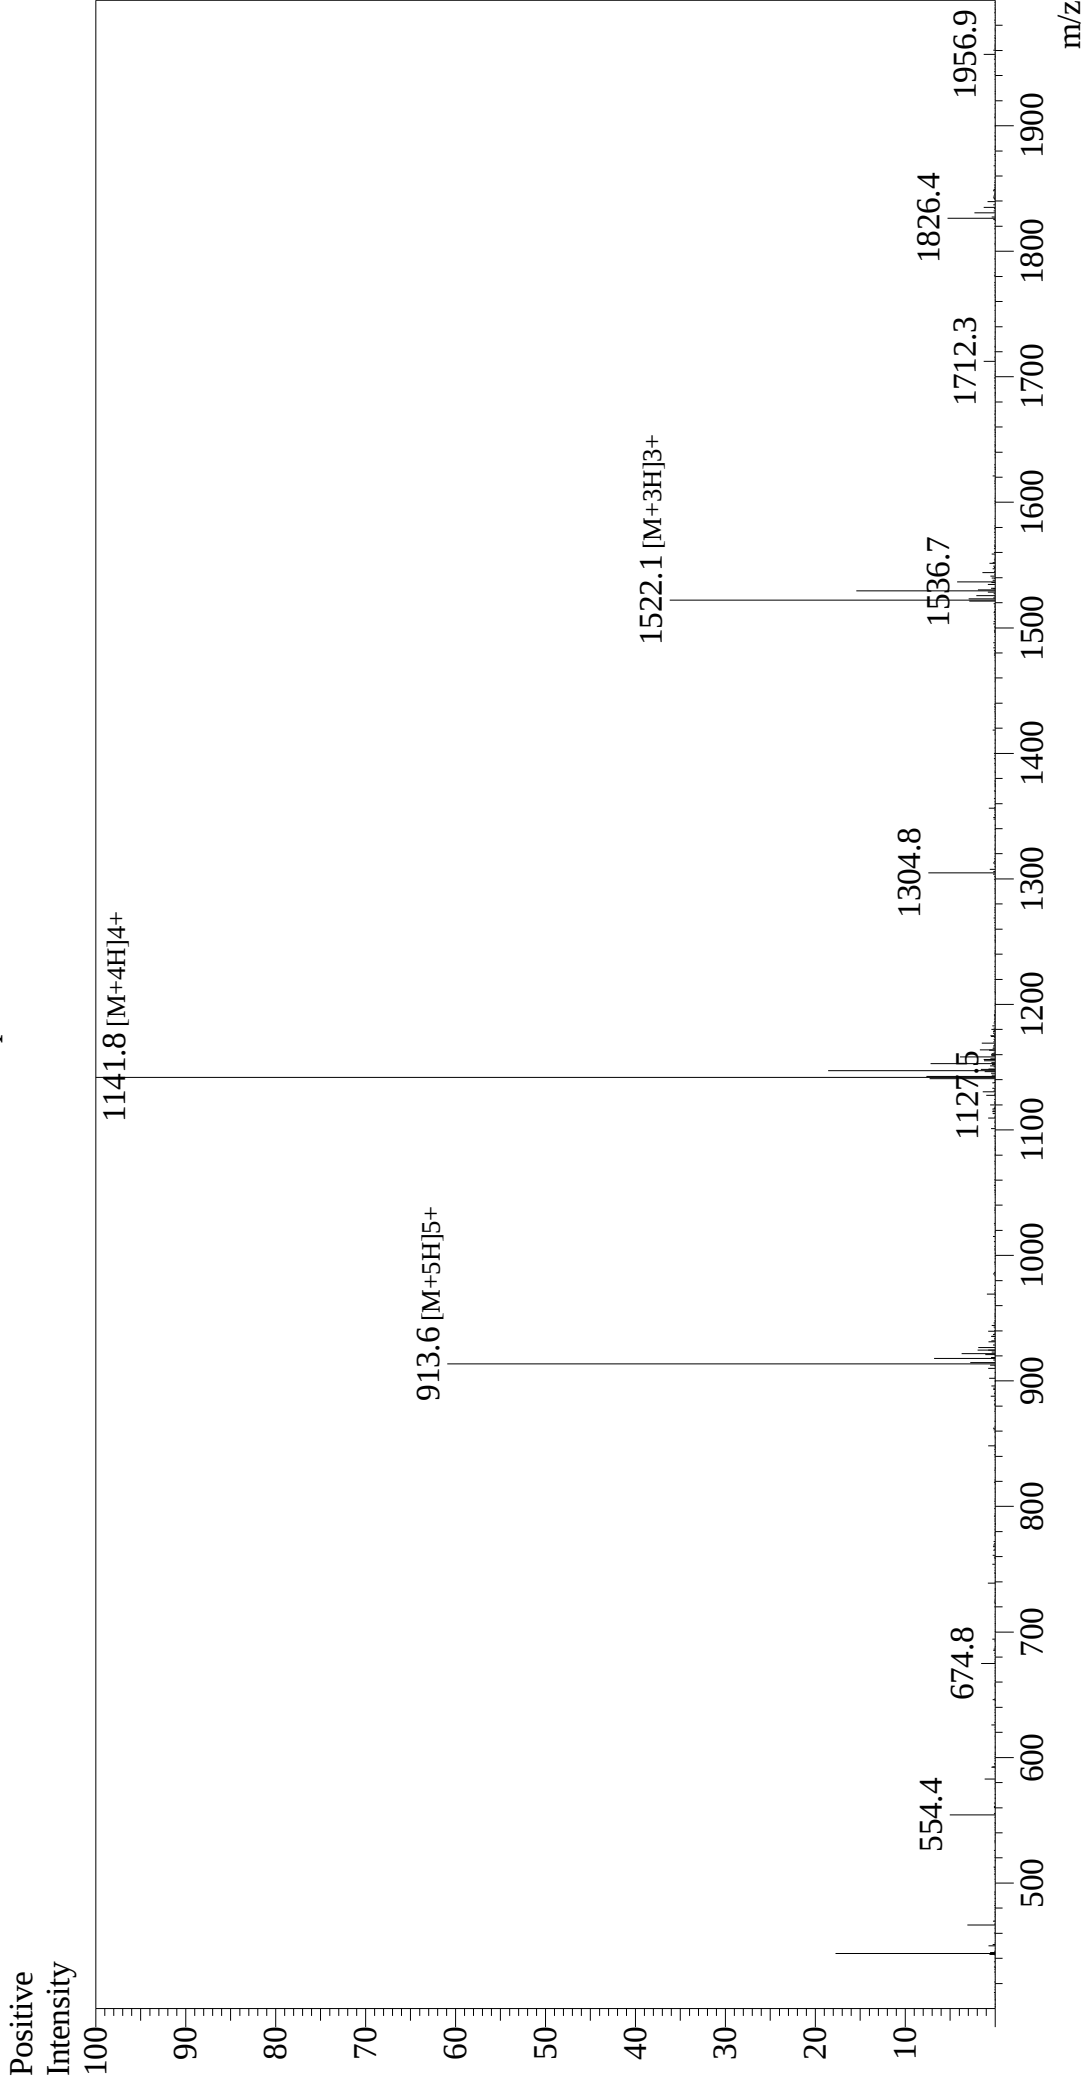

Sample Information

Month-Day Processed : 09/22/25
 Time Processed : 19:49:19
 Injection Volume : 0.3
 Sample Name : [D-SER]33-Mazdutide
 Cat No. : RP30899
 Lot No. : E9747425H
 Theoretical MW : 4563.14
 Observed MW : 4563.2

Interface

Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200

Equipment

Interface Bias : +4.5 kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2 ml/min
 B.conc : 50%H₂O/50%MeOH

Equipment : ZJ22010150