


Mass Spectrum

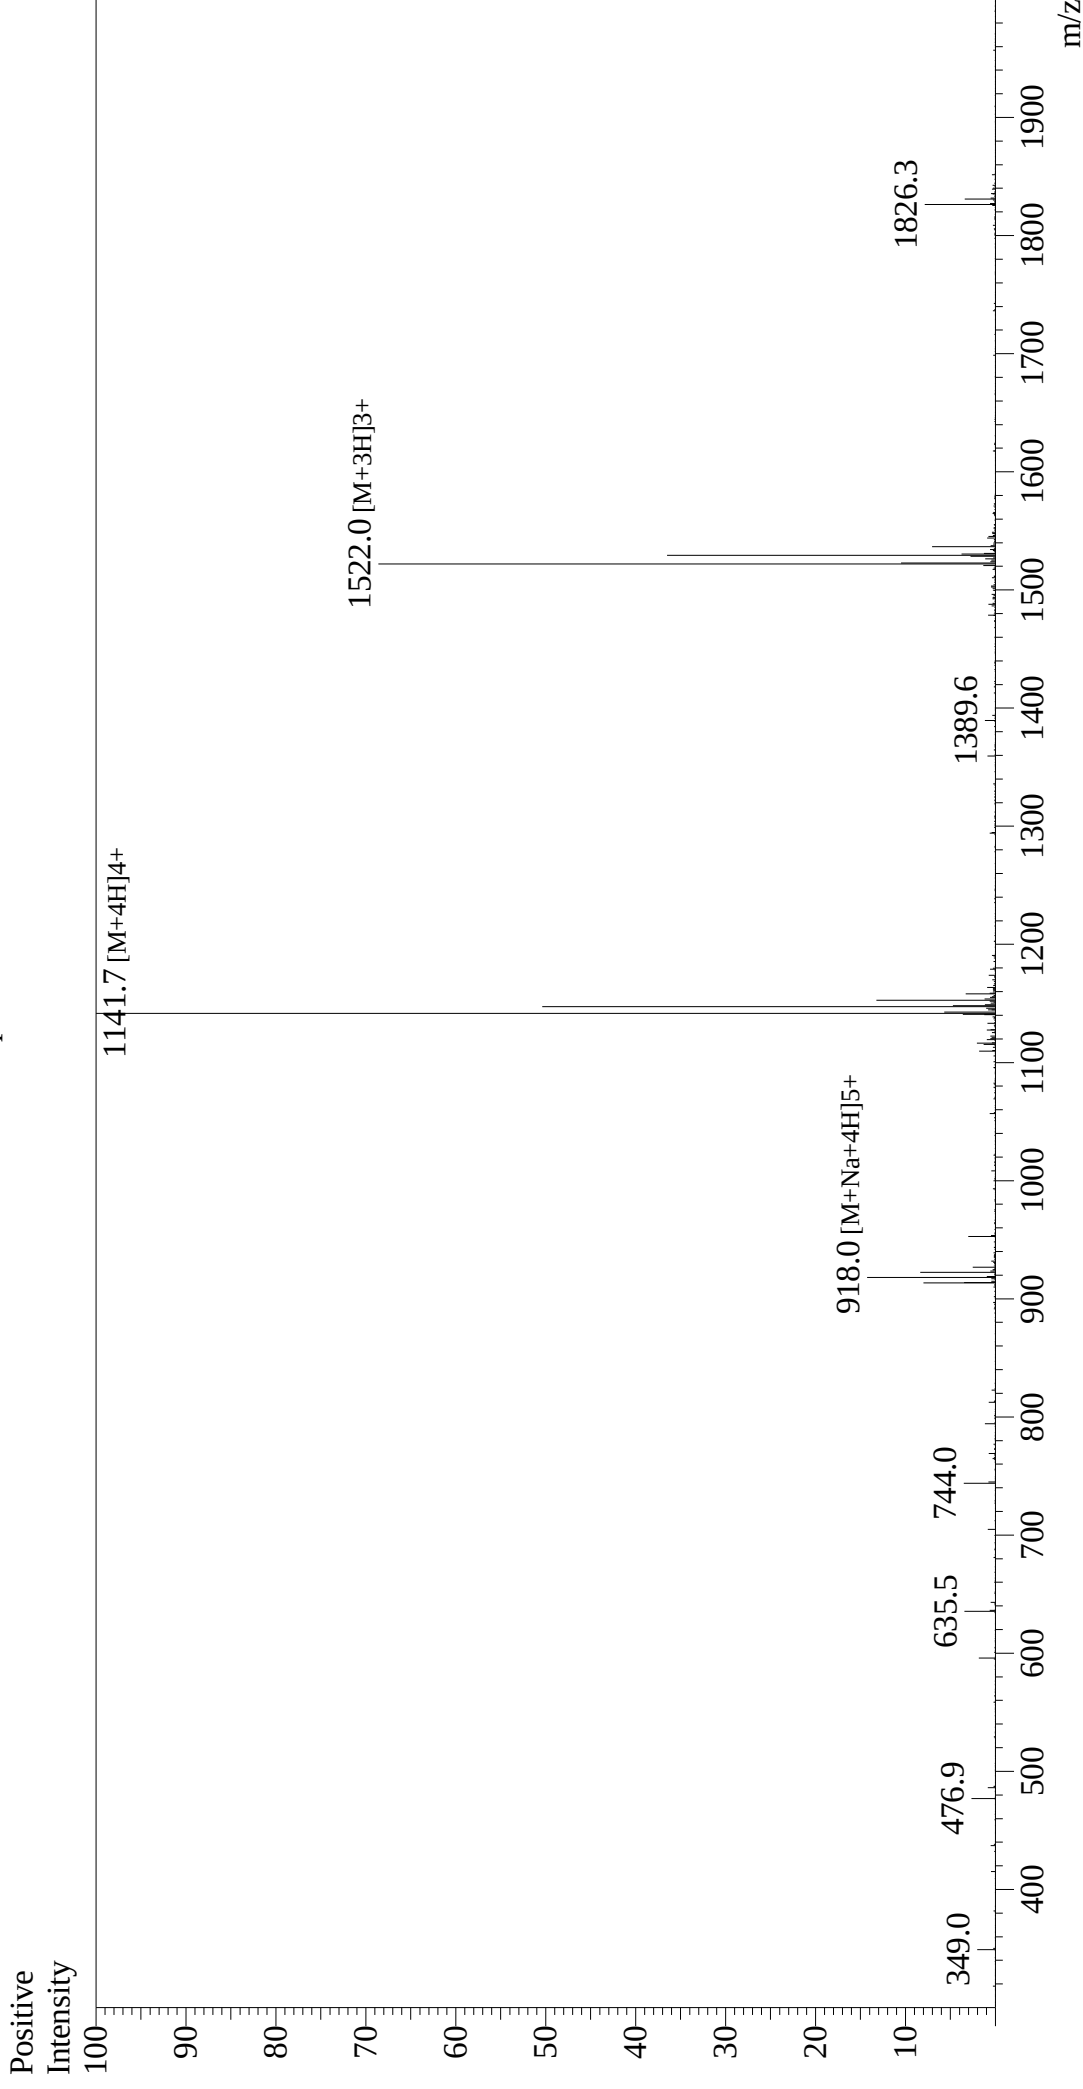

Sample Information

Month-Day Processed : 09/23/25
 Time Processed : 18:25:54
 Injection Volume : 0.3
 Sample Name : [D-GLU]16-Mazdutide
 Cat No. : RP30900
 Lot No. : E9749525H

Theoretical MW: 4563.14

Observed MW : 4562.8

Interface

Interface : ESI
 Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200

Equipment

Equipment : ZJ21010035
 Interface Bias : +4.5 kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2 ml/min
 B.conc : 50%H₂O/50%MeOH