


Mass Spectrum

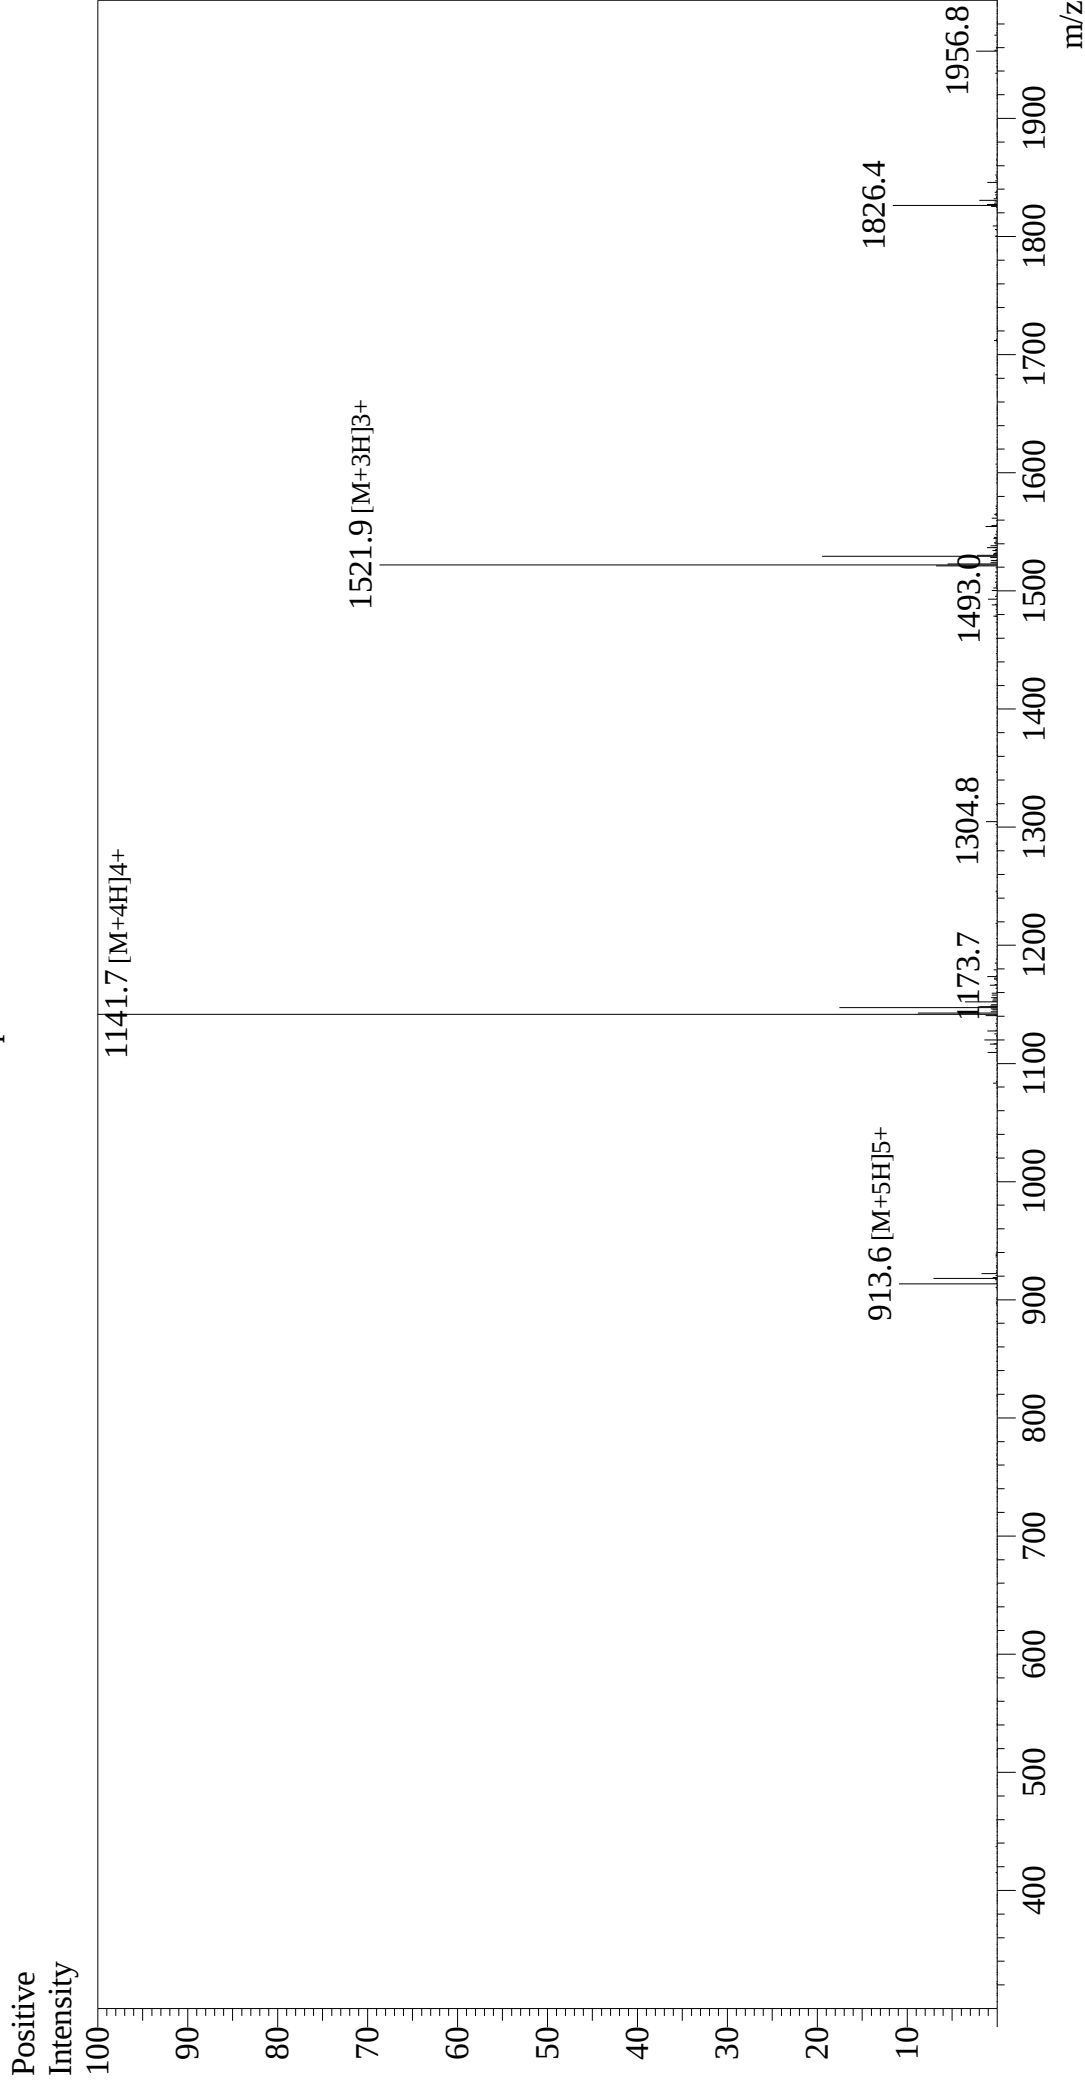

Sample Information

Month-Day Processed : 08/29/25
Time Processed : 18:46:52
Injection Volume : 0.3
Sample Name : [D-GLU]16-Mazdutide
Cat No. : RP30900
Lot No. : E9750325H
Theoretical MW : 4563.14
Observed MW : 4562.8

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : ZJ22010150
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH