


Mass Spectrum

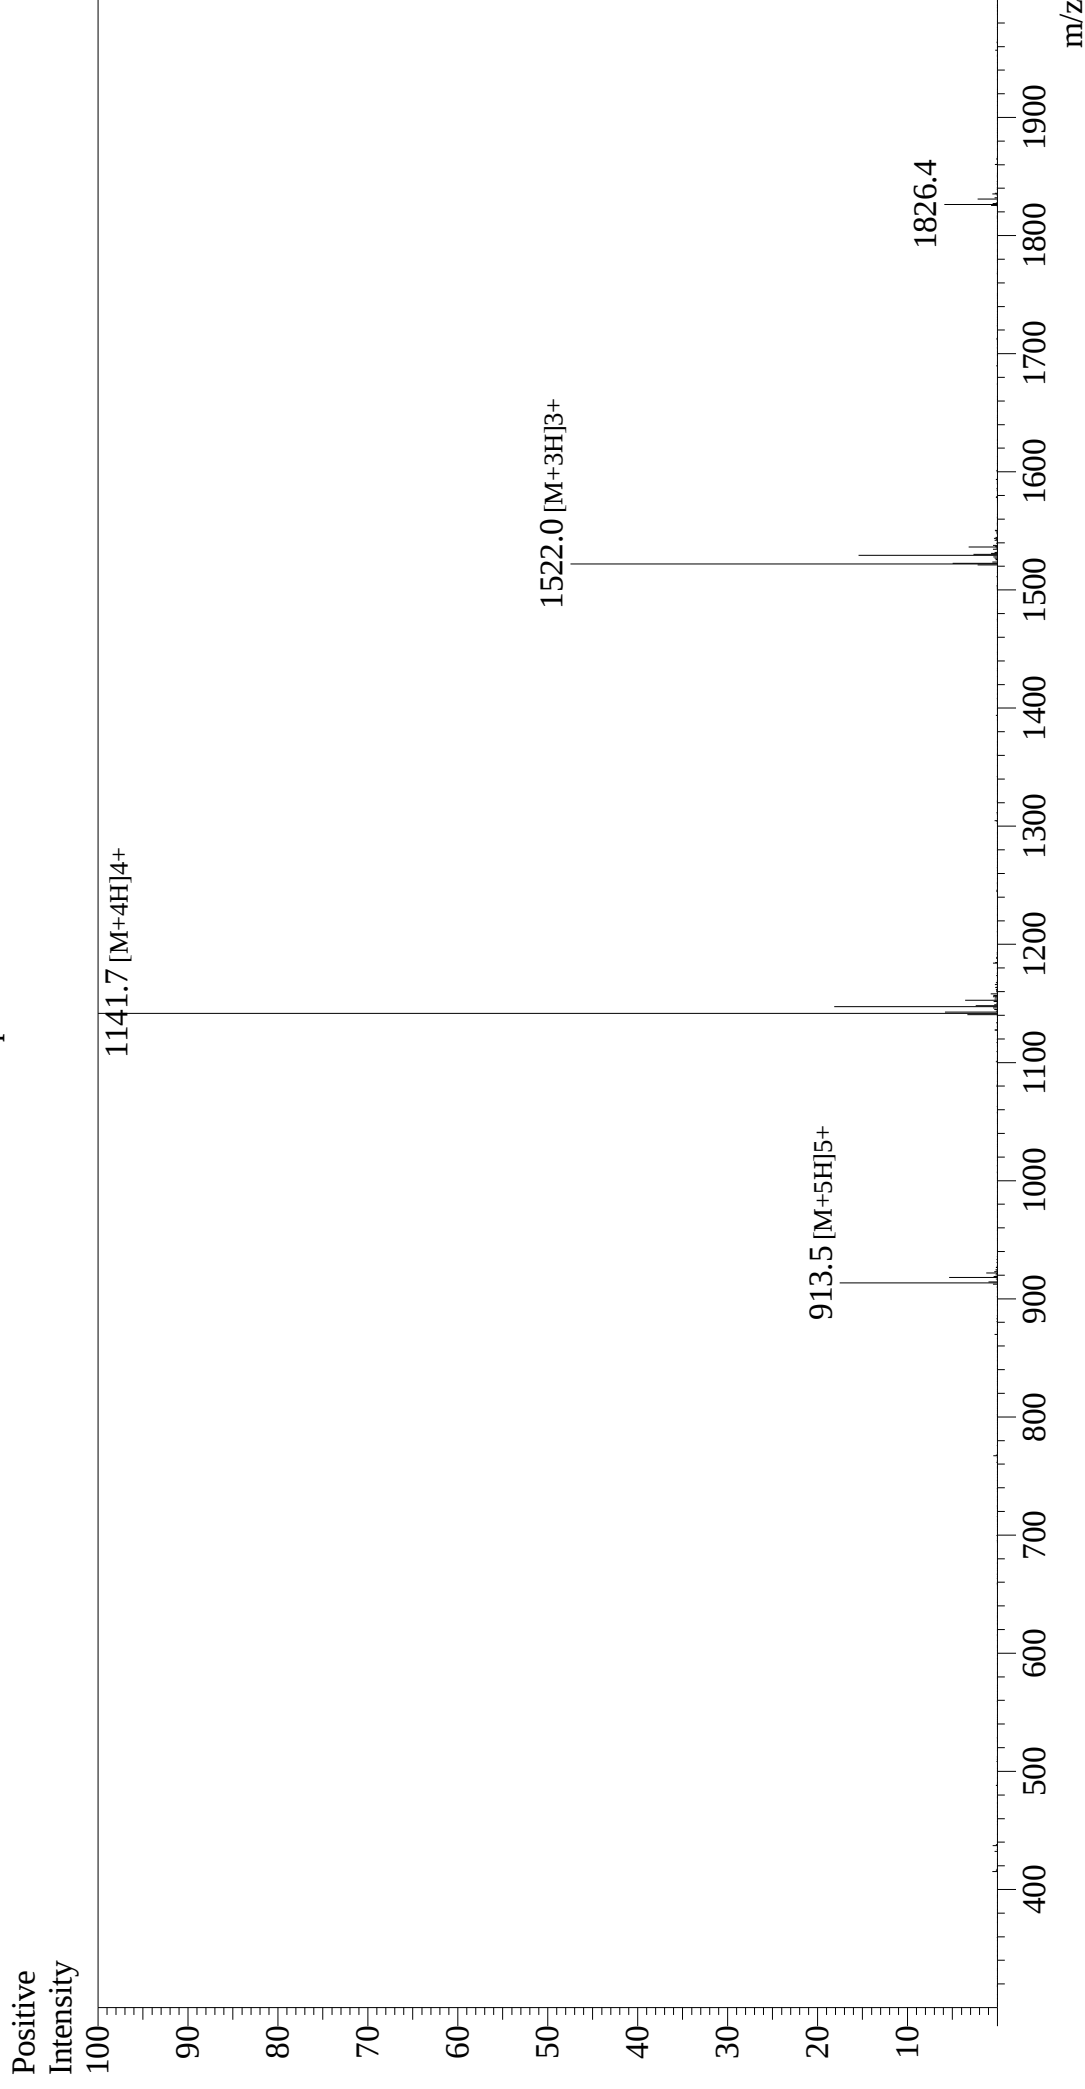

Sample Information

Month-Day Processed : 09/22/25
Time Processed : 19:59:22
Injection Volume : 0.3
Sample Name : [D-ALA]19-Mazdutide
Cat No. : RP30908
Lot No. : E9765225H
Theoretical MW : 4563.14
Observed MW : 4562.8

Interface

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment

Equipment : ZJ21010035
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H₂O/50%MeOH